

Data File : BE093343.D
Acq On : 23 Jun 2017 18:55
Operator : SJ/JU
Sample : I3653-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
F5E21

Quant Time: Jun 24 04:29:24 2017
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 24 04:29:07 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.73	152	1562	0.40	ng/ul	0.00
2) Naphthalene-d8	10.51	136	8480	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.36	164	5445	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.10
16) Chrysene-d12	21.26	240	12238	0.40	ng/ul	0.00
20) Perylene-d12	23.51	264	750361	0.40	ng/ul	-0.15

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.10	152	3935	0.32	ng/ul	0.00
14) Fluoranthene-d10	19.12	212	10325	0.00	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.56	128	7344	0.35	ng/ul#	92
5) 2-Methylnaphthalene	12.18	142	1295	0.09	ng/ul	99
7) Acenaphthylene	14.08	152	376	0.02	ng/ul#	53
8) Acenaphthene	14.42	153	4797	0.25	ng/ul	98
9) Fluorene	15.41	166	9466	0.43	ng/ul	91
17) Pyrene	19.51	202	10027	0.28	ng/ul#	85
18) Benzo(a)anthracene	21.24	228	1903	0.06	ng/ul#	86
19) Chrysene	21.29	228	1755	0.05	ng/ul	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BE093343.D

Acq On : 23 Jun 2017 18:55

Operator : SJ/JU

Sample : I3653-11

Misc :

ALS Vial : 10 Sample Multiplier: 1

Instrument :

BNA_E

ClientSampleId :

F5E21


Quant Time: Jun 24 04:29:24 2017


Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE060717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sat Jun 24 04:29:07 2017

Response via : Initial Calibration

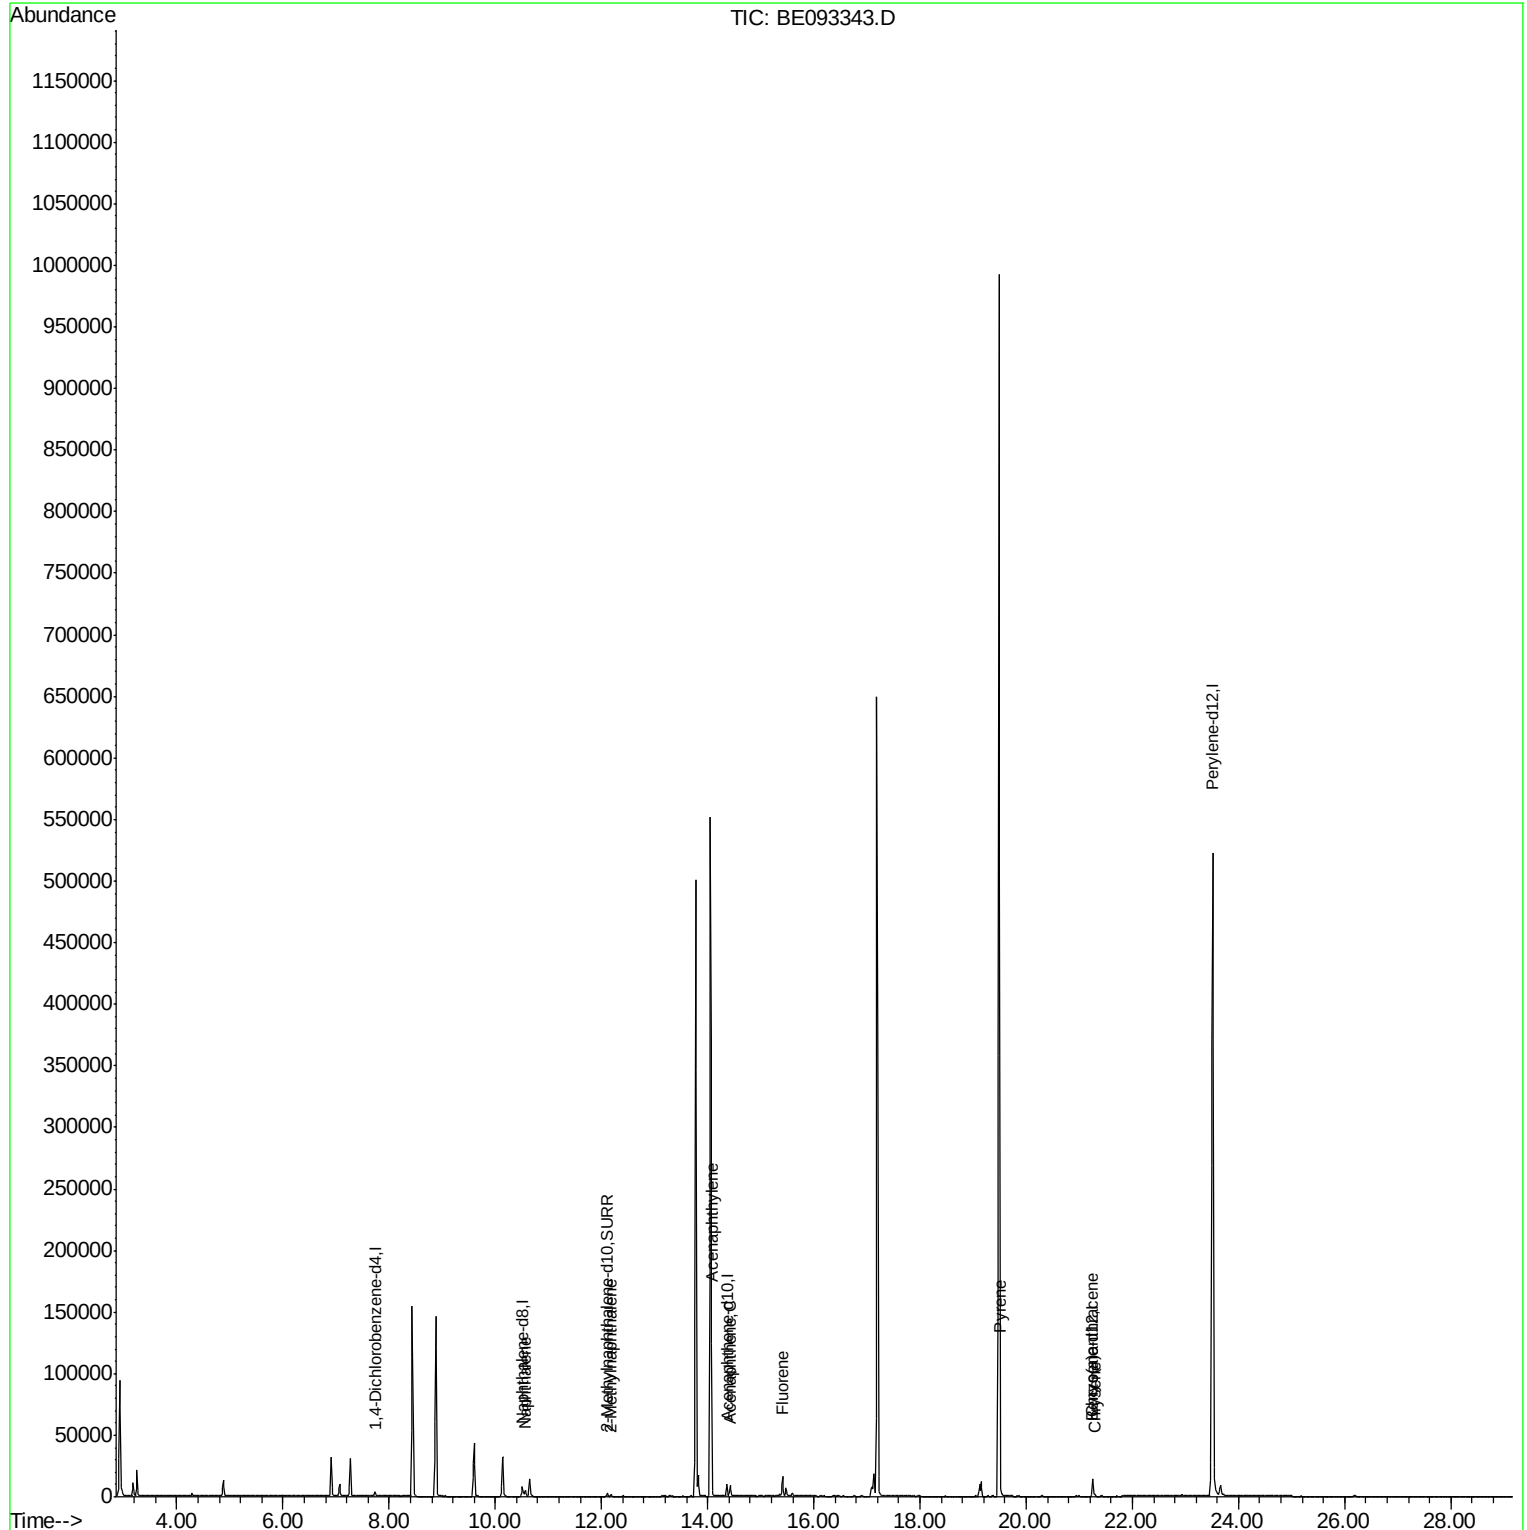

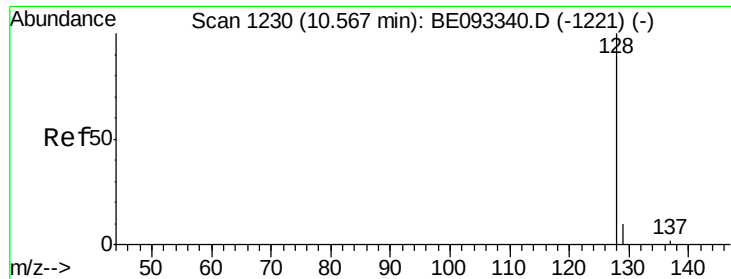

#3

Naphthalene

Concen: 0.35 ng/ul

RT: 10.56 min Scan# 1229

Delta R.T. -0.00 min

Lab File: BE093343.D

Acq: 23 Jun 2017 18:55

Instrument :

BNA_E

ClientSampleId :

F5E21


Tgt Ion:128 Resp: 7344

Ion Ratio Lower Upper

128 100

129 11.9 11.3 16.9




127 0.0 4.0 6.0#

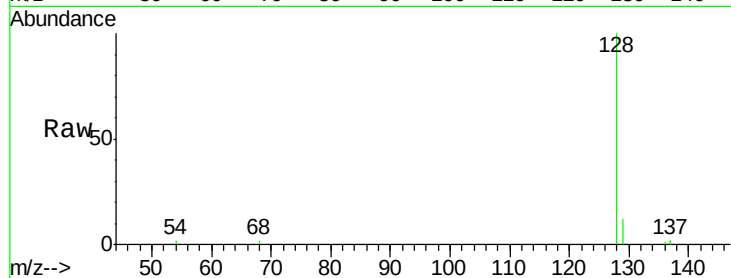

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

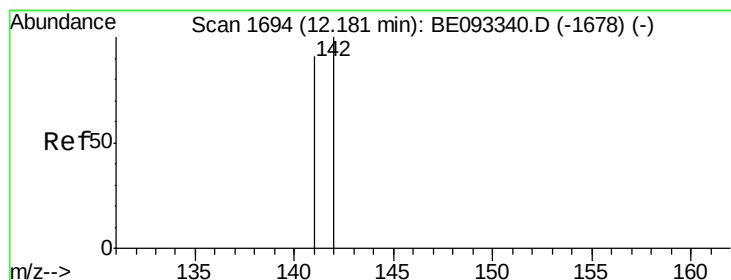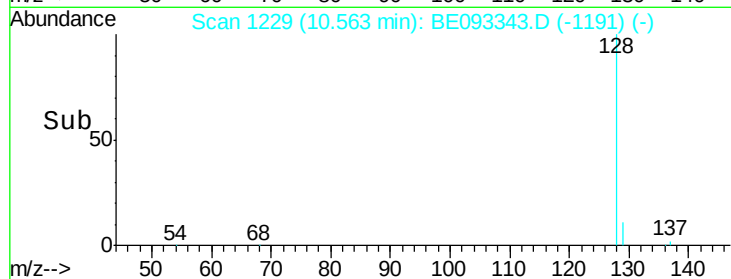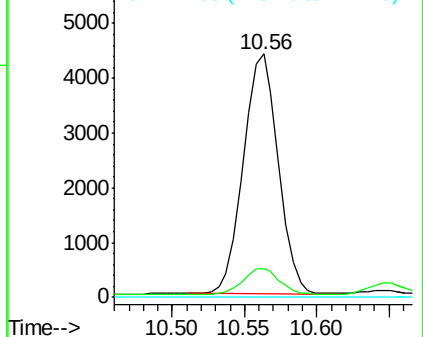

#5

2-Methylnaphthalene

Concen: 0.09 ng/ul

RT: 12.18 min Scan# 1694

Delta R.T. 0.00 min

Lab File: BE093343.D


Acq: 23 Jun 2017 18:55

Tgt Ion:142 Resp: 1295

Ion Ratio Lower Upper



142 100


141 89.6 72.6 108.8

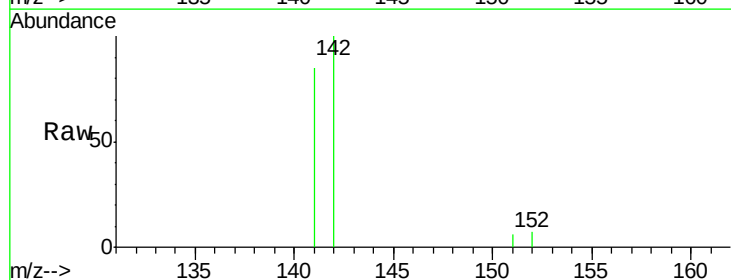

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

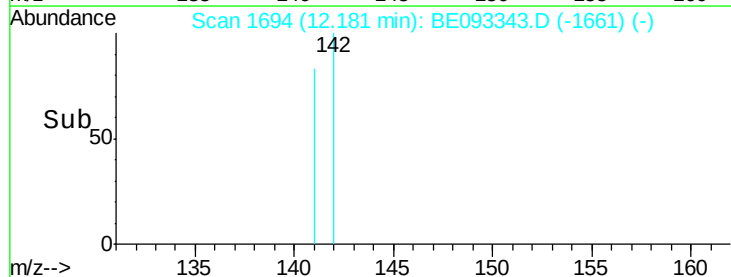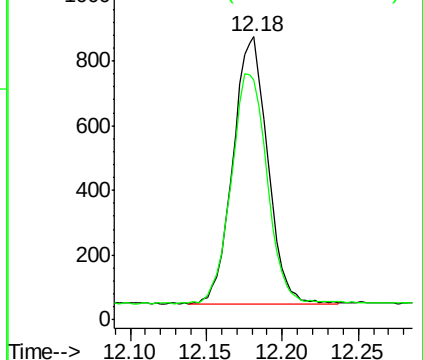

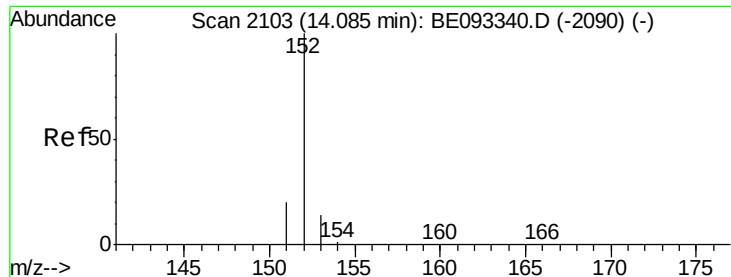

#7

Acenaphthylene

Concen: 0.02 ng/ul

RT: 14.08 min Scan# 2102

Delta R.T. -0.01 min

Lab File: BE093343.D

Acq: 23 Jun 2017 18:55

Instrument :

BNA_E

ClientSampleId :

F5E21


Tgt Ion:152 Resp: 376

Ion Ratio Lower Upper

152 100

151 38.7 17.1 25.7#




153 41.7 12.8 19.2#

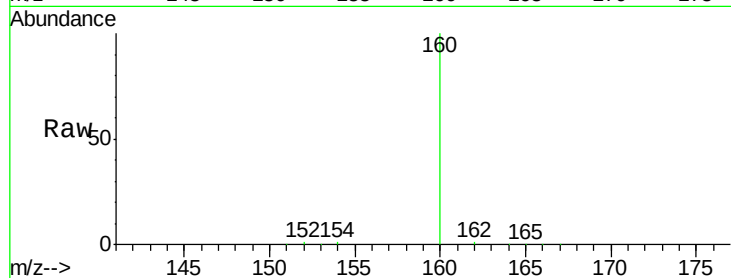

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

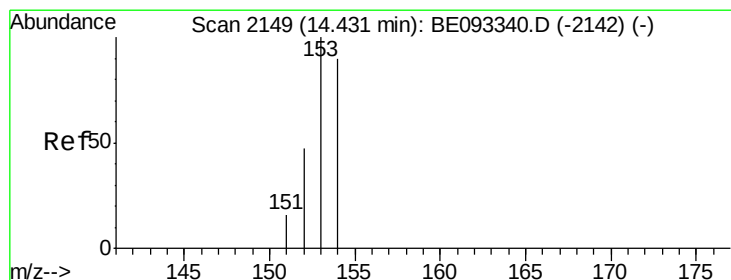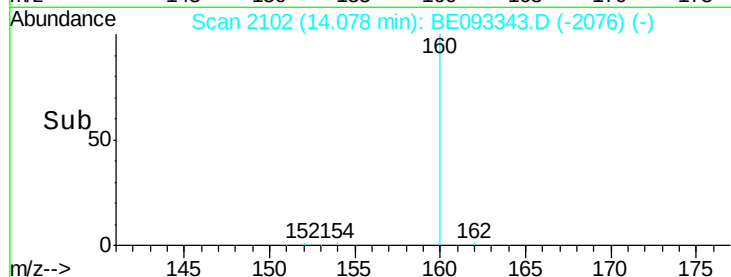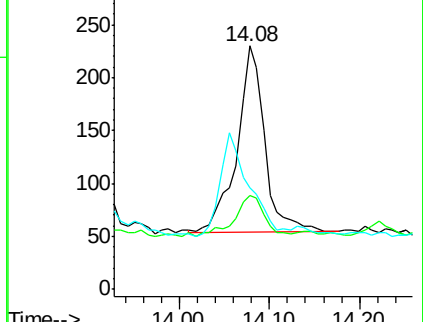

#8

Acenaphthene

Concen: 0.25 ng/ul

RT: 14.42 min Scan# 2148

Delta R.T. -0.01 min

Lab File: BE093343.D

Acq: 23 Jun 2017 18:55


Tgt Ion:153 Resp: 4797

Ion Ratio Lower Upper

153 100

152 49.6 40.3 60.5



154 87.5 71.4 107.2

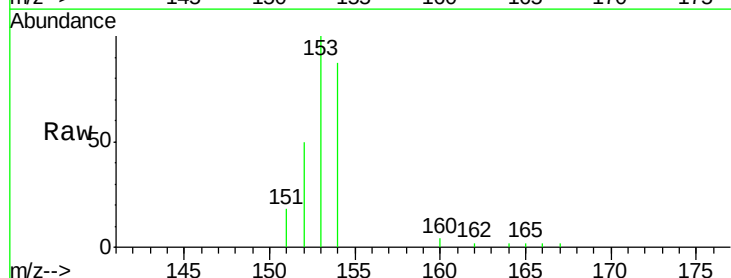


Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

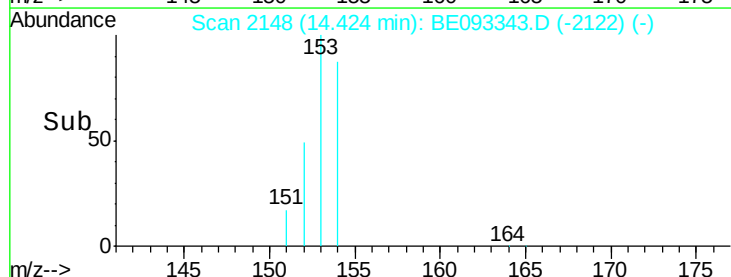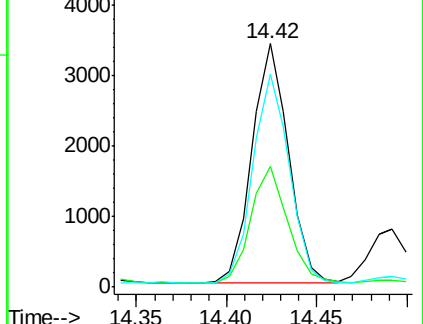

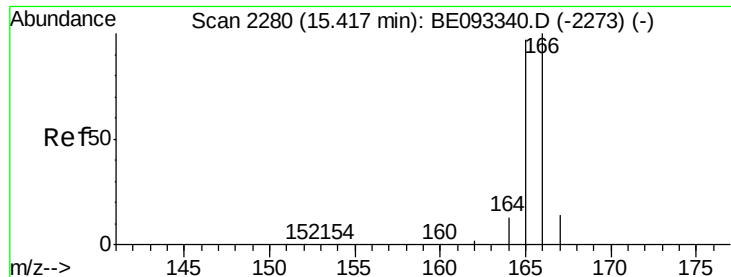

#9

Fluorene

Concen: 0.43 ng/ul

RT: 15.41 min Scan# 2279

Delta R.T. -0.01 min

Lab File: BE093343.D

Acq: 23 Jun 2017 18:55

Instrument :

BNA_E

ClientSampleId :

F5E21





Tgt Ion:166 Resp: 9466

Ion Ratio Lower Upper

166 100

165 100.3 73.4 110.2

167 15.2 14.6 22.0

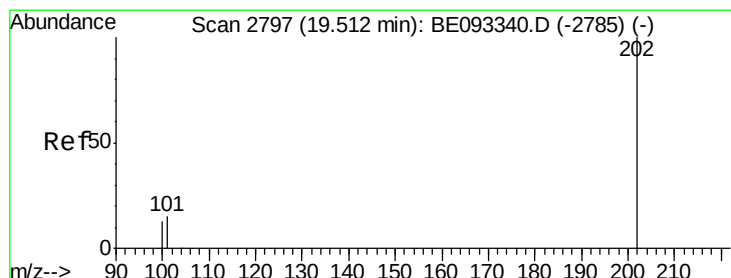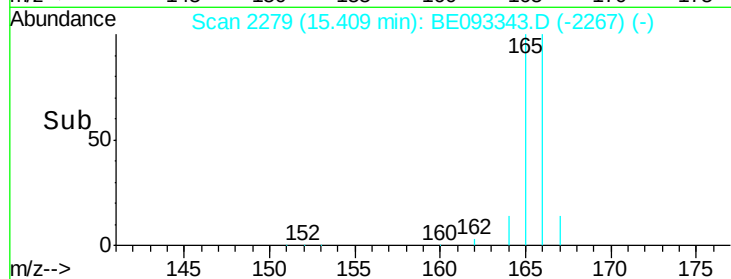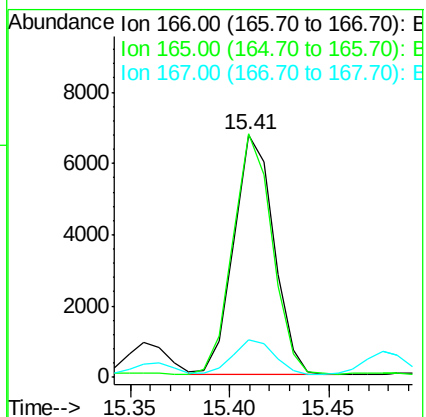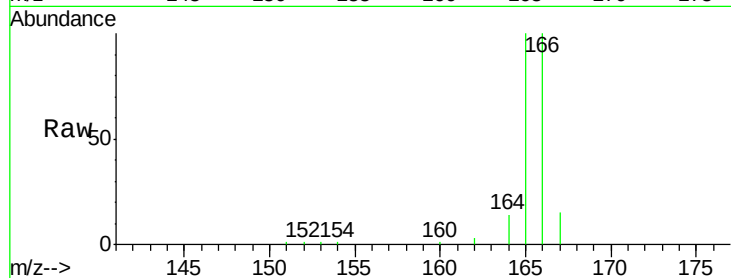

#17

Pyrene

Concen: 0.28 ng/ul

RT: 19.51 min Scan# 2798

Delta R.T. 0.00 min

Lab File: BE093343.D

Acq: 23 Jun 2017 18:55




Tgt Ion:202 Resp: 10027


Ion Ratio Lower Upper

202 100

101 15.7 18.2 27.4#

100 12.9 15.6 23.4#

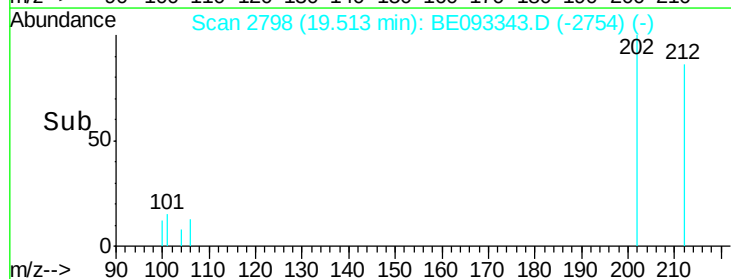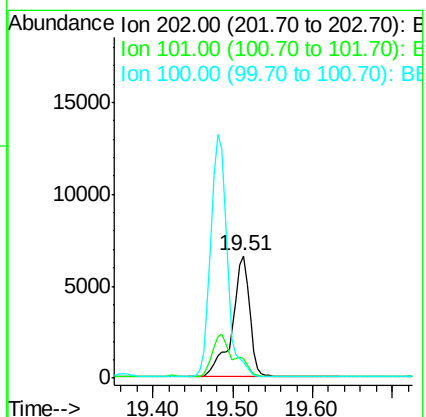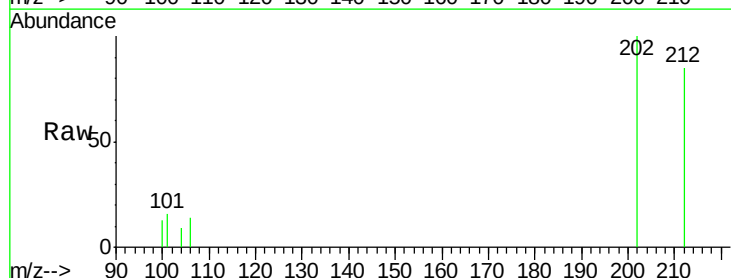

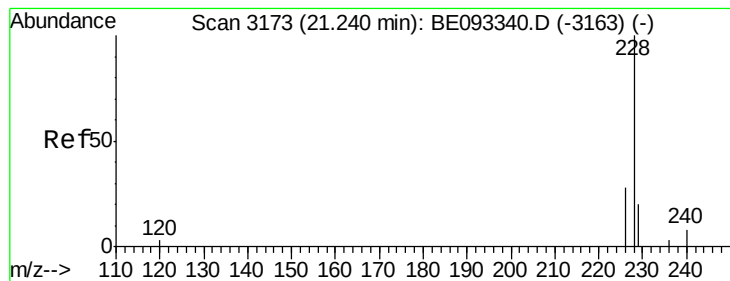

#18

Benzo(a)anthracene

Concen: 0.06 ng/ul

RT: 21.24 min Scan# 3174

Delta R.T. 0.00 min

Lab File: BE093343.D

Acq: 23 Jun 2017 18:55

Instrument :

BNA_E

ClientSampleId :

F5E21


Tgt Ion:228 Resp: 1903

Ion Ratio Lower Upper




228 100

229 22.6 22.8 34.2#

226 29.2 17.0 25.6#

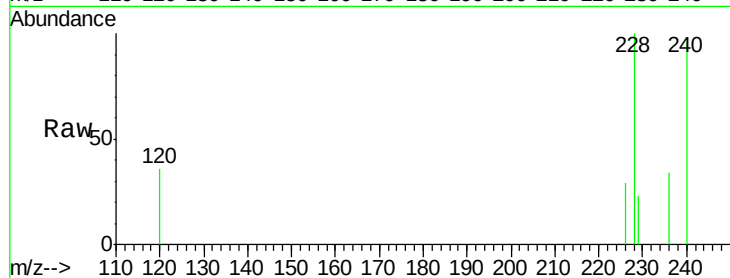

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

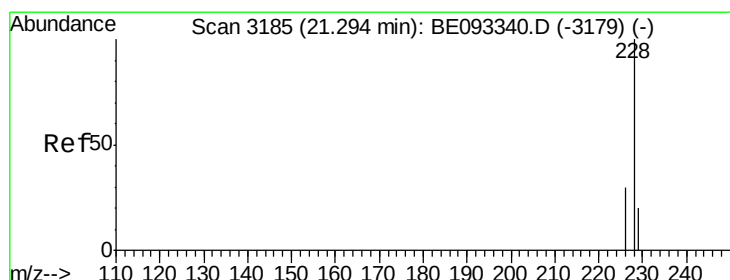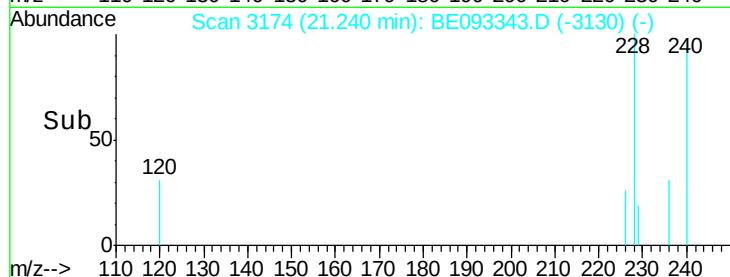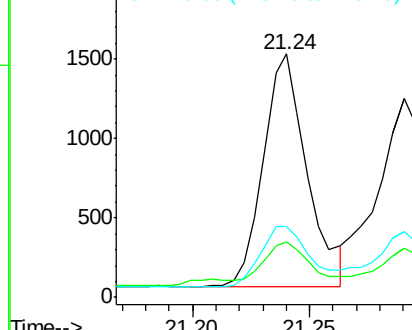

#19

Chrysene

Concen: 0.05 ng/ul

RT: 21.29 min Scan# 3185

Delta R.T. -0.00 min

Lab File: BE093343.D

Acq: 23 Jun 2017 18:55


Tgt Ion:228 Resp: 1755

Ion Ratio Lower Upper

228 100

226 33.4 23.4 35.0

229 24.7 17.7 26.5

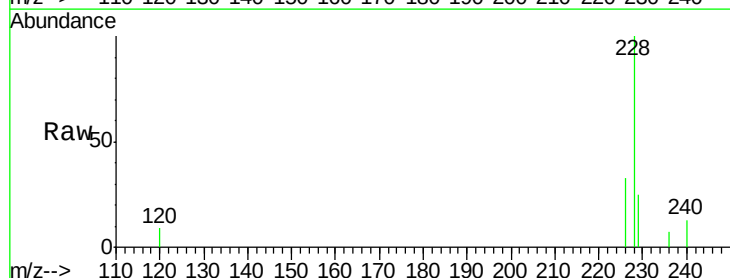

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

