


Data Path : Z:\HPCHEM1\BNA_E\Data\BE062415\
 Data File : BE089932.D
 Acq On : 24 Jun 2015 13:55
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BE062315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 25 16:51:27 2015

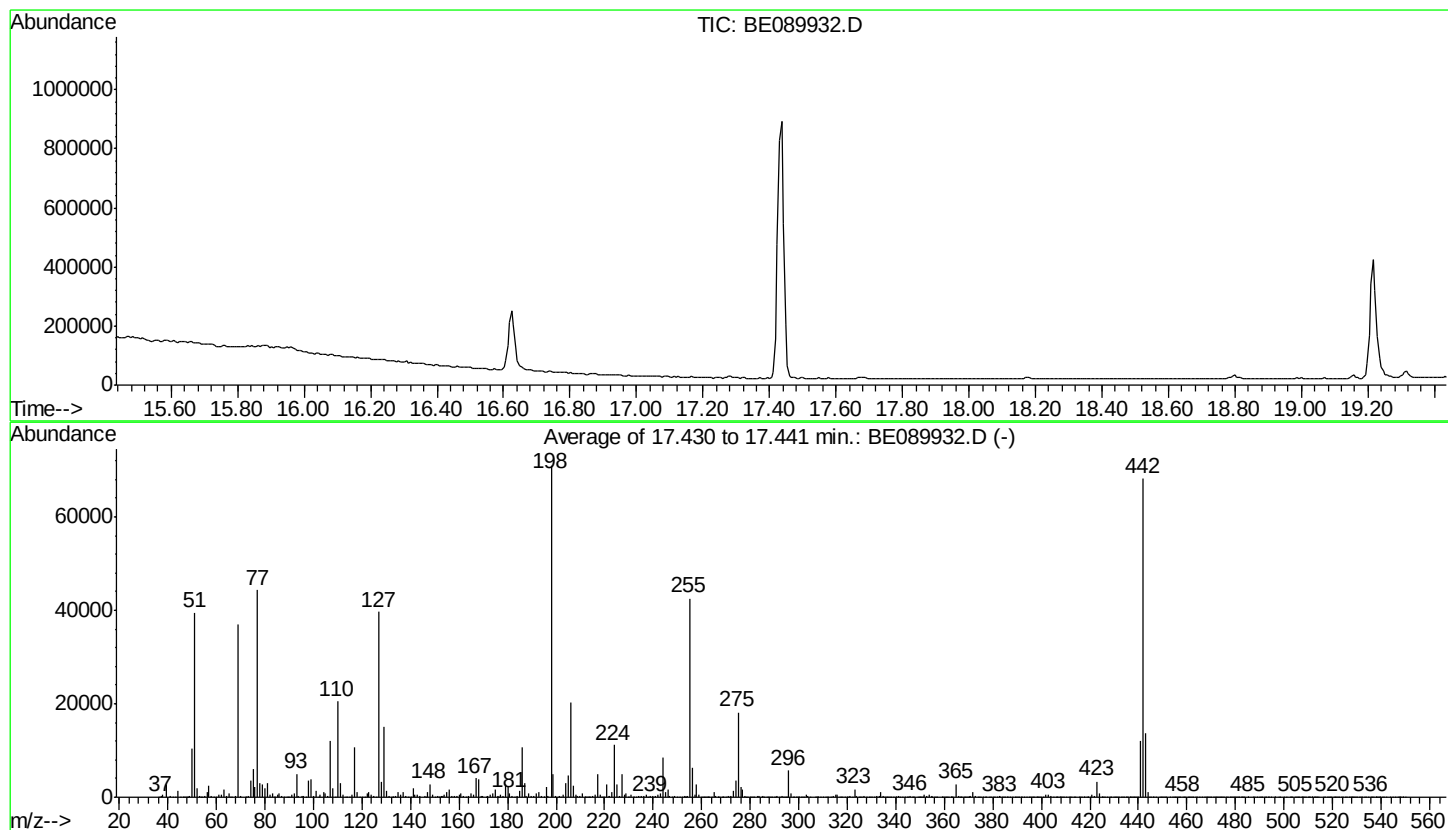

AutoFind: Scans 2526, 2527, 2528; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.6	39491	PASS
68	69	0.00	2	0.7	263	PASS
69	198	0.00	100	52.0	36911	PASS
70	69	0.00	2	0.9	314	PASS
127	198	10	80	55.8	39645	PASS
197	198	0.00	2	0.2	177	PASS
198	198	100	100	100.0	70988	PASS
199	198	5	9	6.9	4894	PASS
275	198	10	60	25.5	18137	PASS
365	198	1	100	3.9	2767	PASS
441	442	0.01	24	17.6	11997	PASS
442	198	50	100	96.0	68136	PASS
443	442	15	24	20.3	13827	PASS