
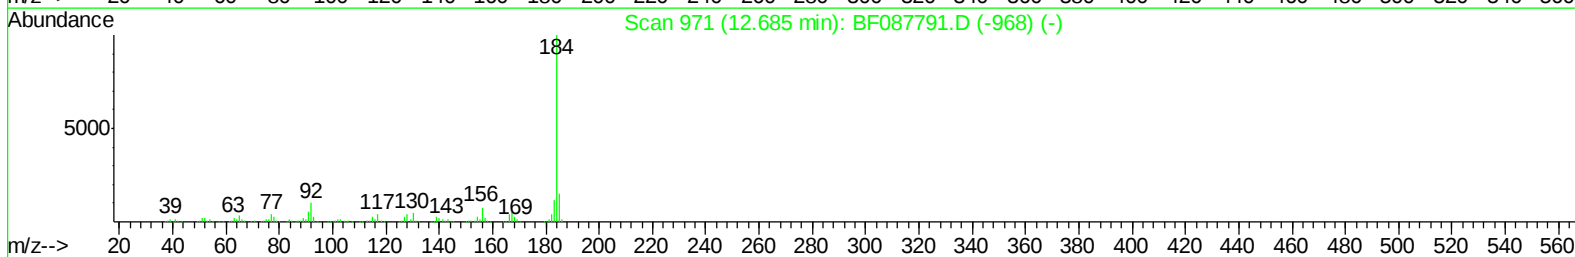
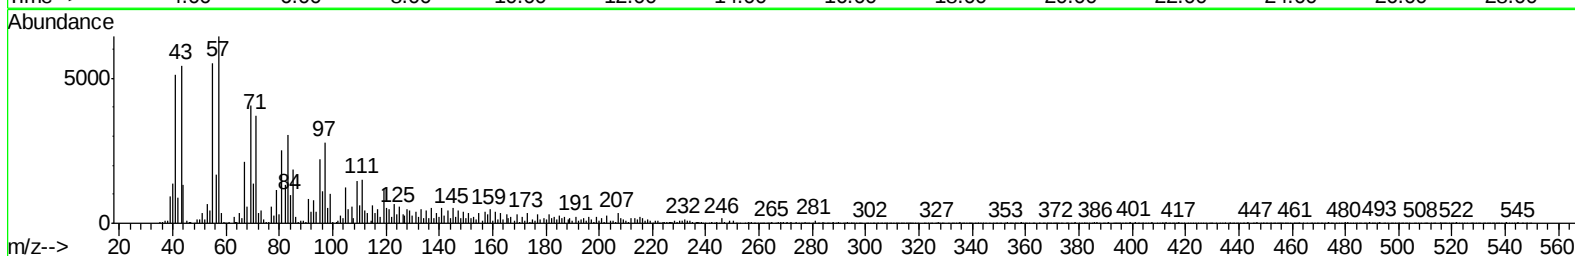


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE062416\
Data File : BE091941.D
Acq On : 24 Jun 2016 9:53
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 23:12:36 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 14:55:14 2016
Response via : Initial Calibration

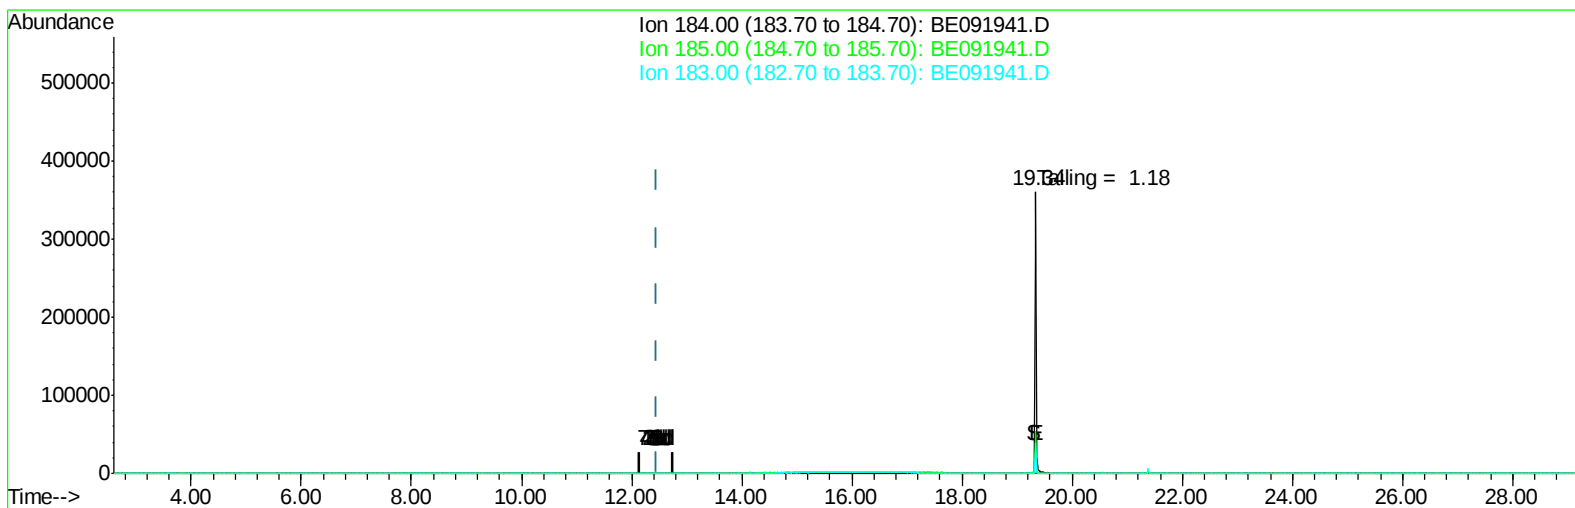

TIC: BE091941.D

(76) Benzidine




12.455min (-0.001) 33.08ng

response 98

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	161.94#
183.00	11.60	129.68#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE062416\
Data File : BE091941.D
Acq On : 24 Jun 2016 9:53
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 24 23:12:36 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF060716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 22 14:55:14 2016
Response via : Initial Calibration

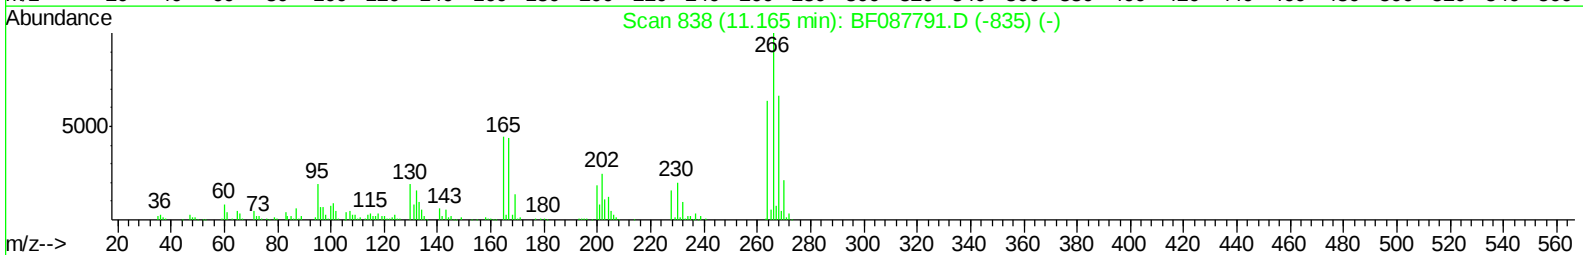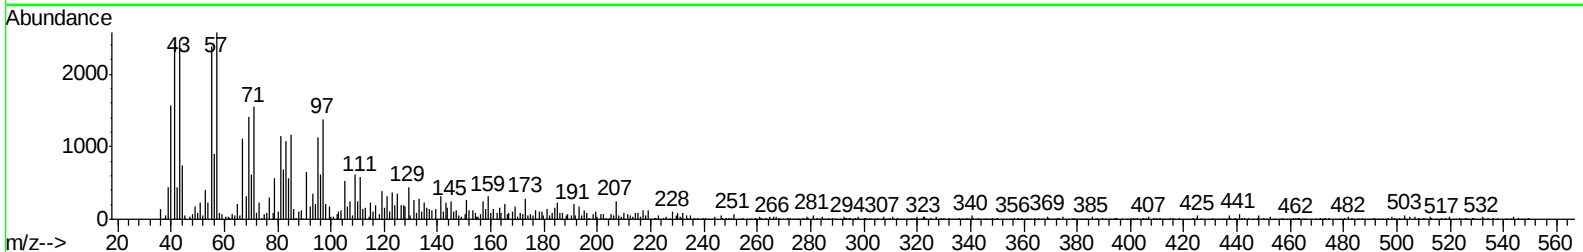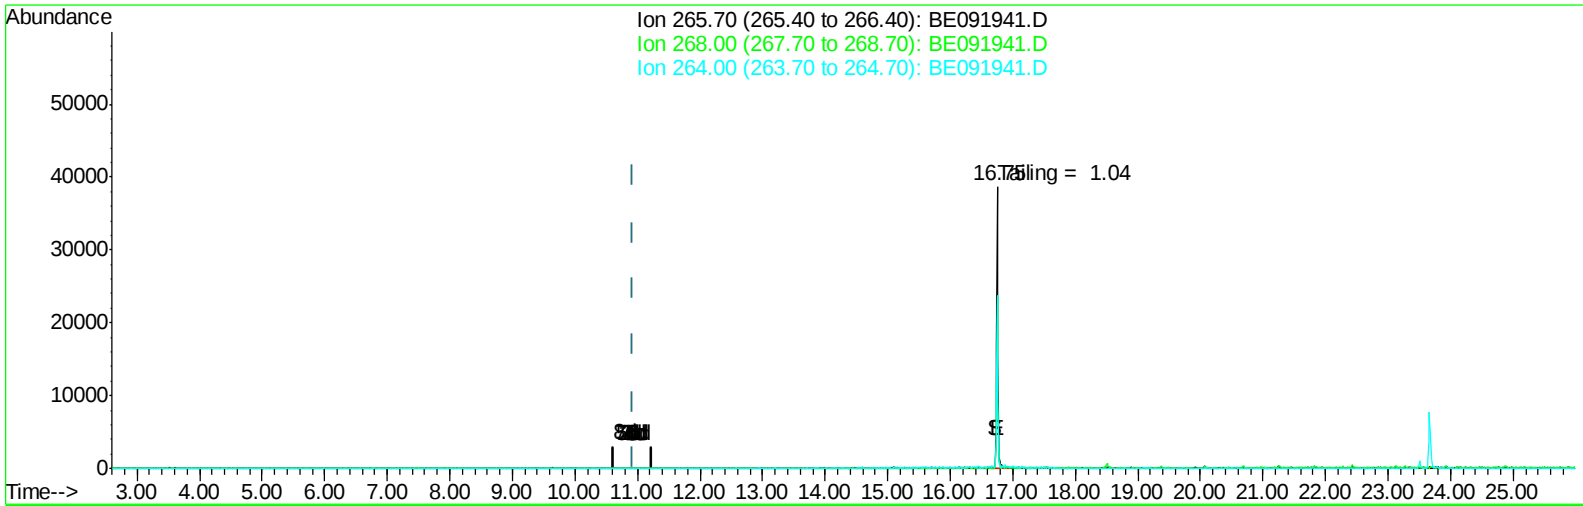

TIC: BE091941.D

(69) Pentachlorophenol (C)

10.910min (-0.026) 60.28ng

response 17

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	56.76
264.00	62.00	8.11#
0.00	0.00	0.00