


Data Path : Z:\HPCHEM1\BNA E\DATA\BE062416\
 Data File : BE091941.D
 Acq On : 24 Jun 2016 9:53
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE061416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 15 12:00:38 2016

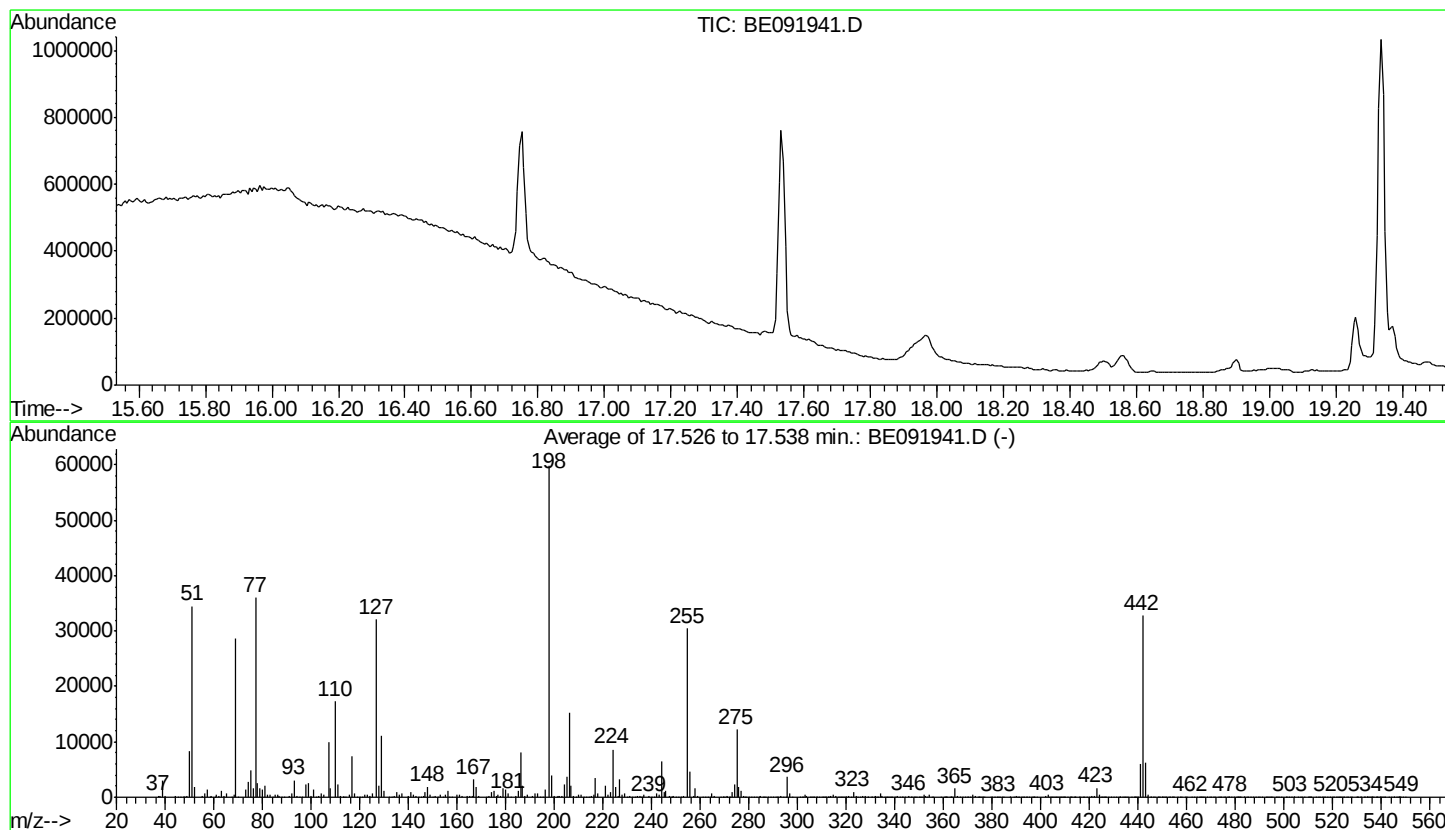

AutoFind: Scans 2542, 2543, 2544; Background Corrected with Scan 2536

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.6	34469	PASS
68	69	0.00	2	1.6	470	PASS
69	198	0.00	100	48.1	28782	PASS
70	69	0.00	2	0.2	65	PASS
127	198	10	80	53.6	32120	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59873	PASS
199	198	5	9	6.7	4001	PASS
275	198	10	60	20.3	12144	PASS
365	198	1	100	2.6	1530	PASS
441	442	0.01	24	18.1	5925	PASS
442	198	50	100	54.8	32800	PASS
443	442	15	24	18.9	6189	PASS