


Data Path : Z:\HPCHEM1\BNA\_E\DATA\BE062615\  
 Data File : BE089941.D  
 Acq On : 26 Jun 2015 12:34  
 Operator : TP/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_M\METHODS\8270-SIM-BE062315.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Jun 25 16:51:27 2015

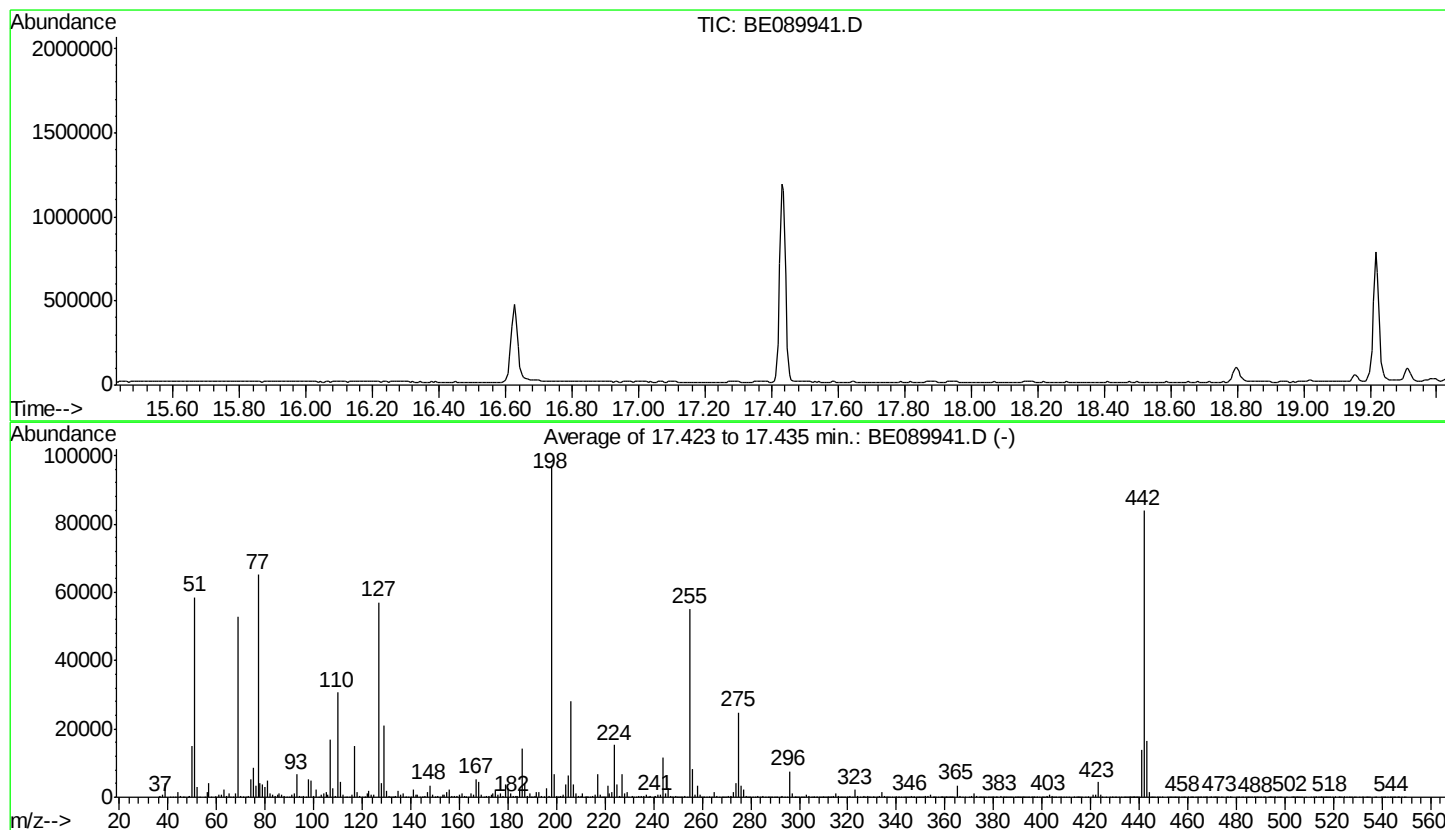

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2518

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 60.4      | 58602   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.8       | 961     | PASS             |
| 69          | 198          | 0.00         | 100          | 54.6      | 52995   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 302     | PASS             |
| 127         | 198          | 10           | 80           | 58.8      | 57085   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.3       | 245     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 97061   | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 6593    | PASS             |
| 275         | 198          | 10           | 60           | 25.6      | 24842   | PASS             |
| 365         | 198          | 1            | 100          | 3.5       | 3417    | PASS             |
| 441         | 442          | 0.01         | 24           | 16.4      | 13740   | PASS             |
| 442         | 198          | 50           | 100          | 86.3      | 83770   | PASS             |
| 443         | 442          | 15           | 24           | 19.6      | 16452   | PASS             |