


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE062615\
 Data File : BE089954.D
 Acq On : 26 Jun 2015 23:12
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BE062315.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 25 16:51:27 2015

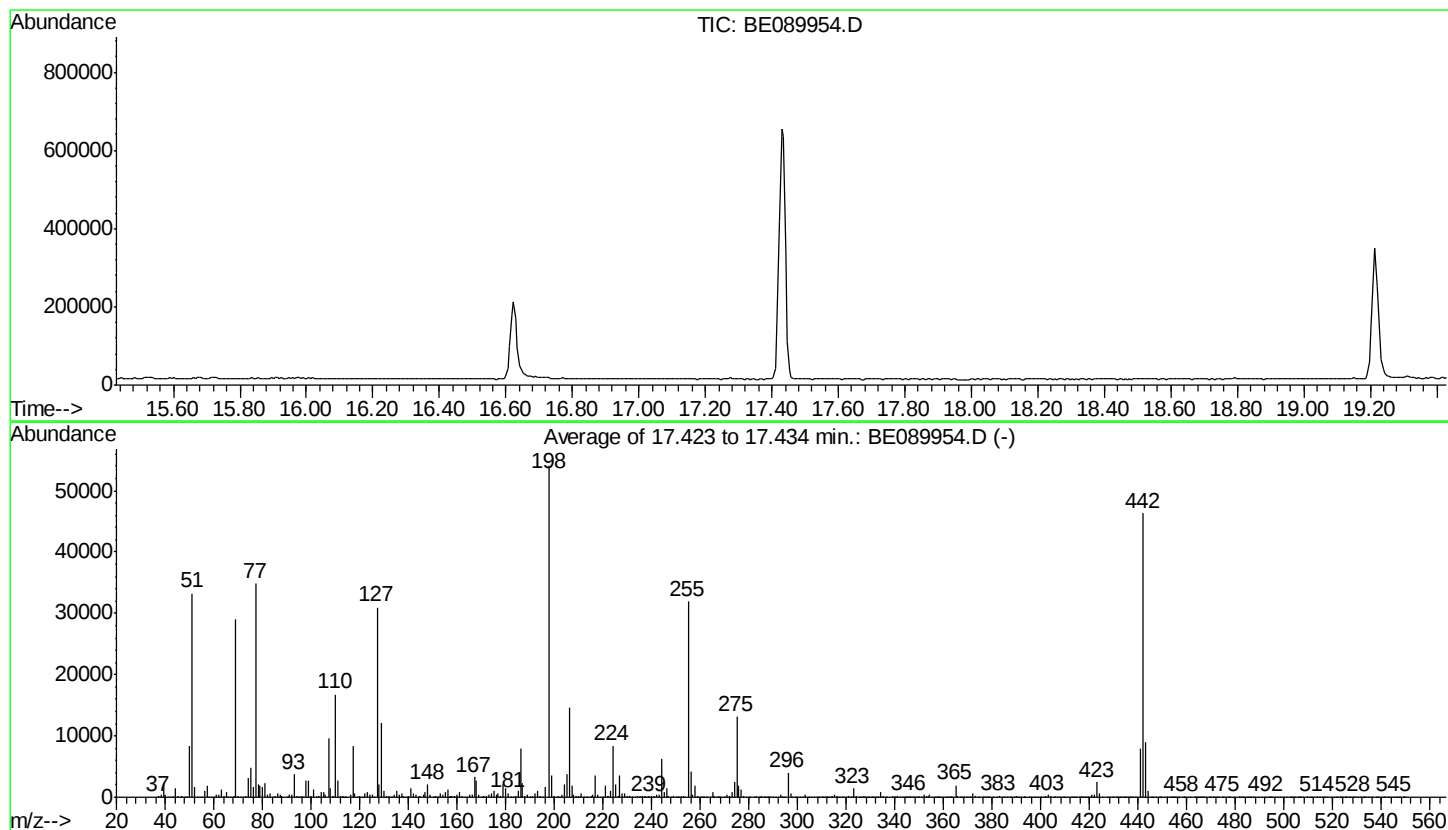

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.5	33278	PASS
68	69	0.00	2	0.7	196	PASS
69	198	0.00	100	53.7	29065	PASS
70	69	0.00	2	0.8	231	PASS
127	198	10	80	57.1	30906	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54090	PASS
199	198	5	9	6.7	3614	PASS
275	198	10	60	24.3	13128	PASS
365	198	1	100	3.6	1961	PASS
441	442	0.01	24	17.3	8019	PASS
442	198	50	100	85.6	46302	PASS
443	442	15	24	19.3	8924	PASS