


Data Path : Z:\HPCHEM1\BNA_E\Data\BE062615\
Data File : BE089963.D
Acq On : 27 Jun 2015 5:46
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BE062315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jun 25 16:51:27 2015

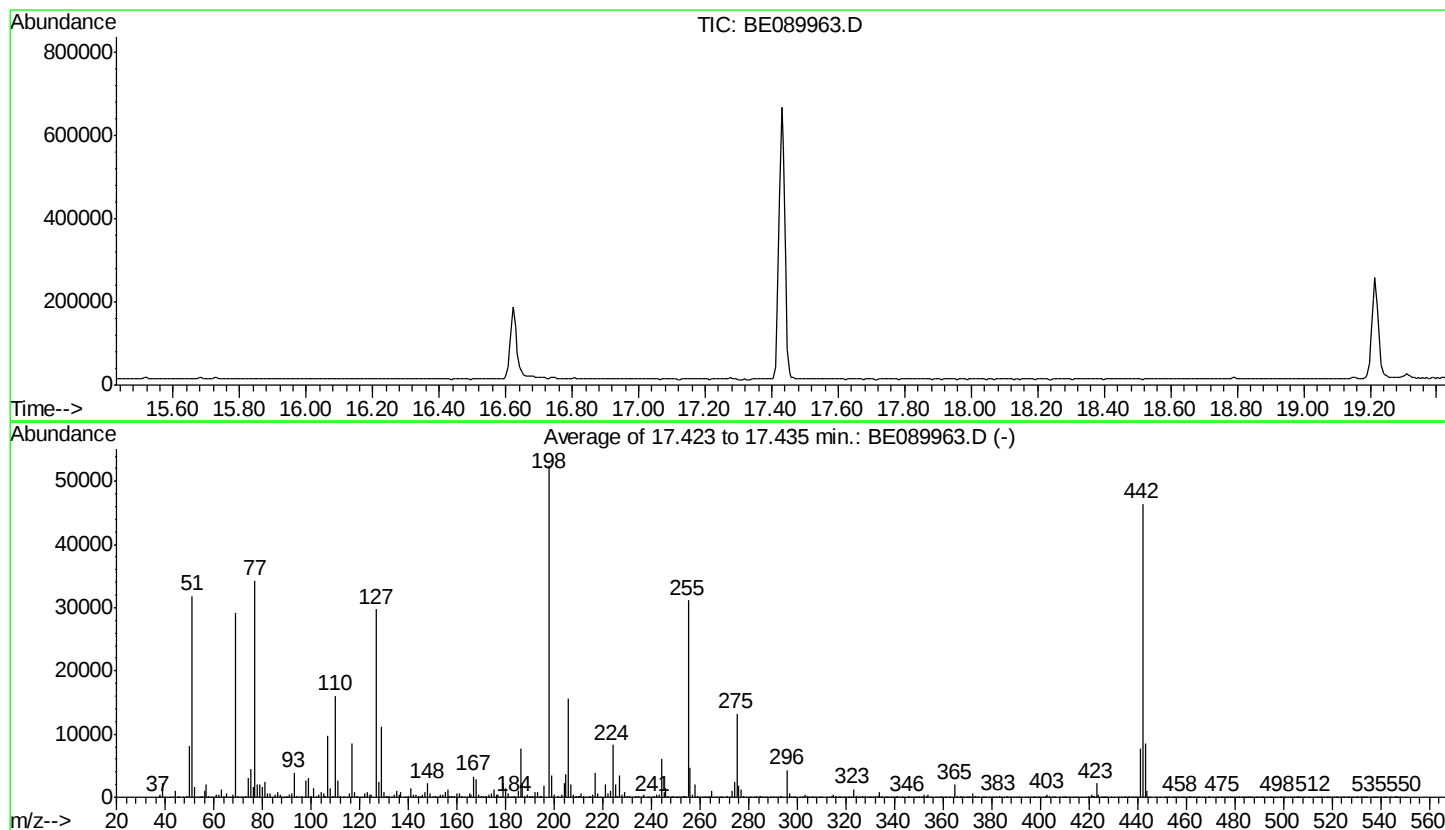

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.8	31917	PASS
68	69	0.00	2	1.6	475	PASS
69	198	0.00	100	55.6	29200	PASS
70	69	0.00	2	0.5	145	PASS
127	198	10	80	56.7	29744	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52490	PASS
199	198	5	9	6.6	3485	PASS
275	198	10	60	25.1	13193	PASS
365	198	1	100	3.8	2017	PASS
441	442	0.01	24	16.8	7806	PASS
442	198	50	100	88.5	46469	PASS
443	442	15	24	18.5	8611	PASS