
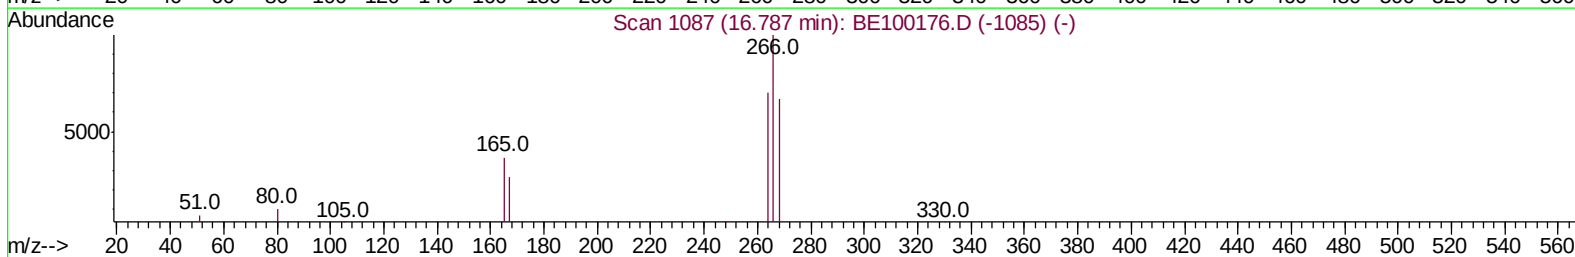
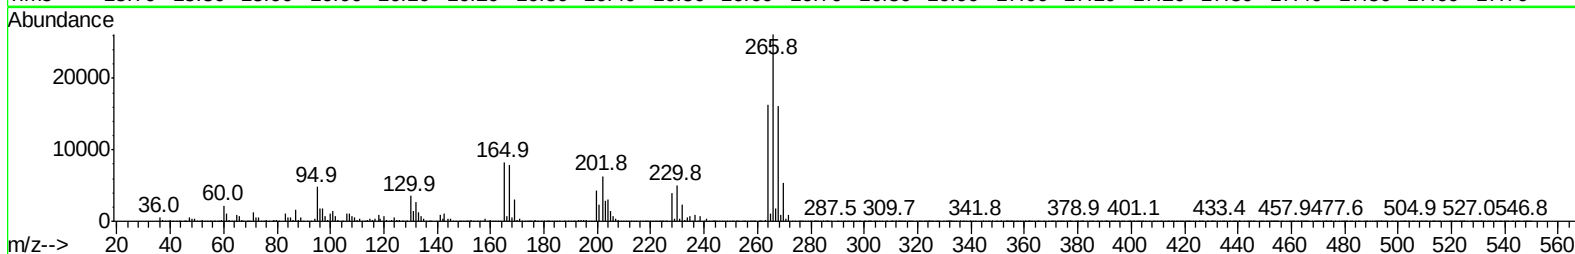


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE062719\
 Data File : BE100207.D
 Acq On : 27 Jun 2019 16:39
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 28 07:09:13 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE062519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 28 05:41:07 2019
 Response via : Initial Calibration

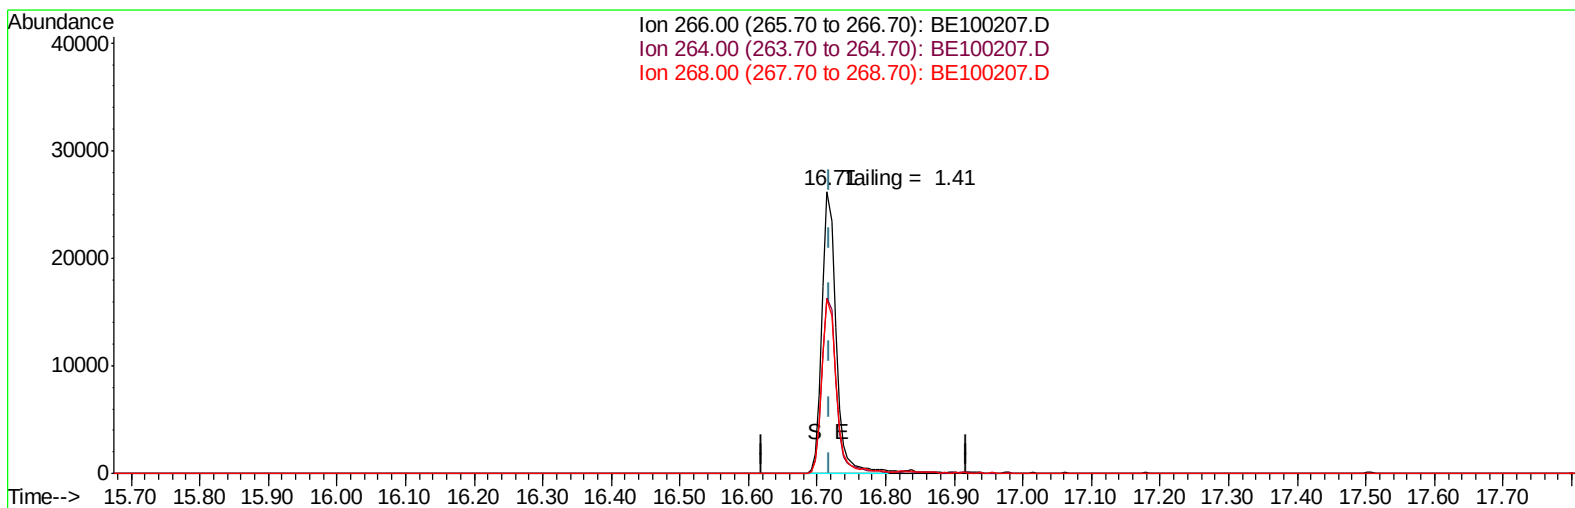

TIC: BE100207.D

(22) Pentachlorophenol

16.715min (-0.004) 157.77ng

response 37095

Ion	Exp%	Act%
266.00	100	100
264.00	84.60	58.47#
268.00	87.20	61.53#
0.00	0.00	0.00