


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE062719\
 Data File : BE100197.D
 Acq On : 27 Jun 2019 9:34
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE062519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 28 05:41:07 2019

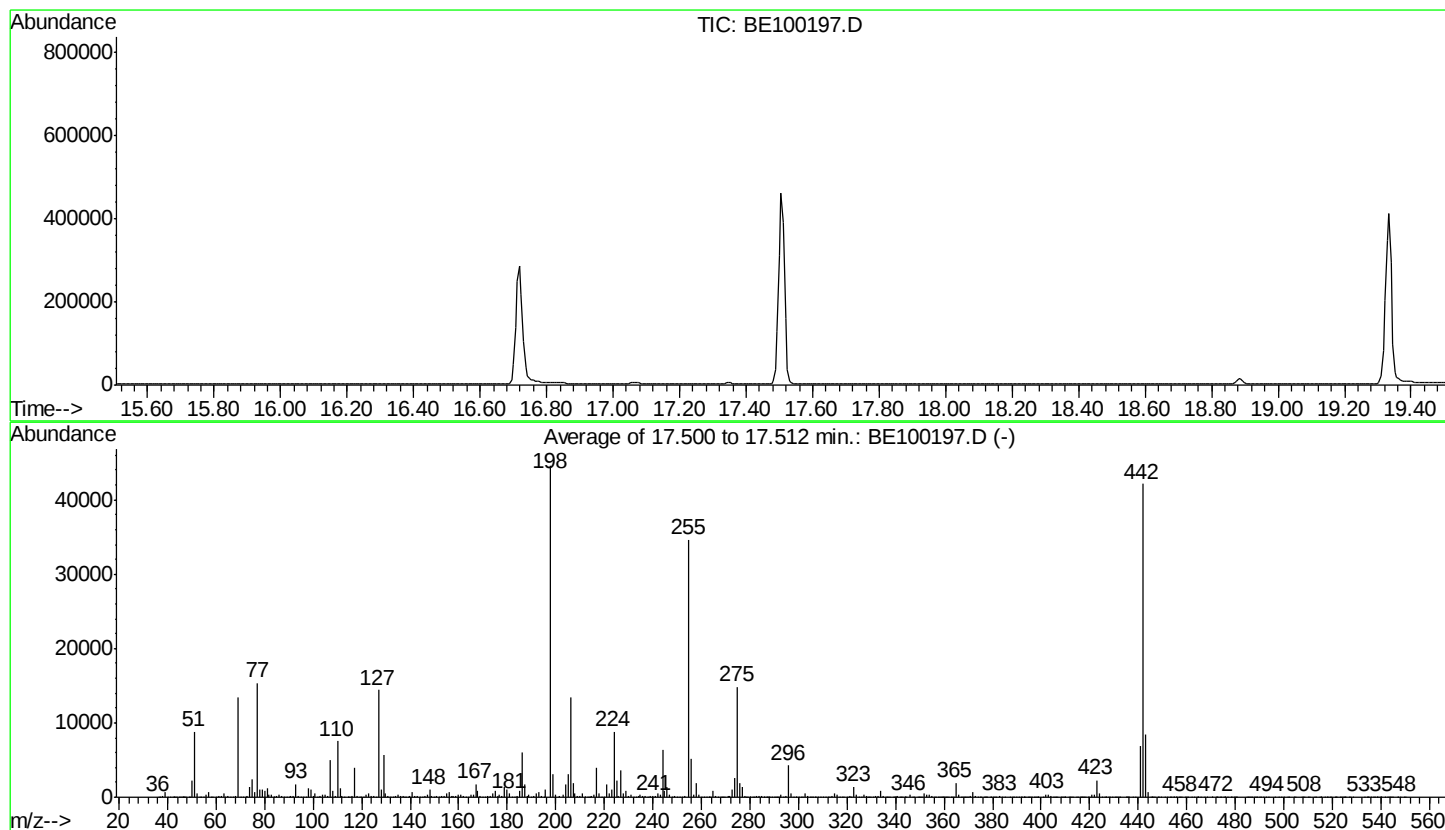

AutoFind: Scans 2538, 2539, 2540; Background Corrected with Scan 2529

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.7	8784	PASS
68	69	0.00	2	1.5	199	PASS
69	198	0.00	100	30.1	13437	PASS
70	69	0.00	2	0.5	62	PASS
127	198	10	80	32.4	14426	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	44593	PASS
199	198	5	9	6.9	3059	PASS
275	198	10	60	33.4	14887	PASS
365	198	1	100	4.3	1905	PASS
441	198	0.01	100	15.3	6807	PASS
442	198	50	100	94.4	42114	PASS
443	442	15	24	20.0	8443	PASS