


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE062719\
 Data File : BE100207.D
 Acq On : 27 Jun 2019 16:39
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE062519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 28 05:41:07 2019

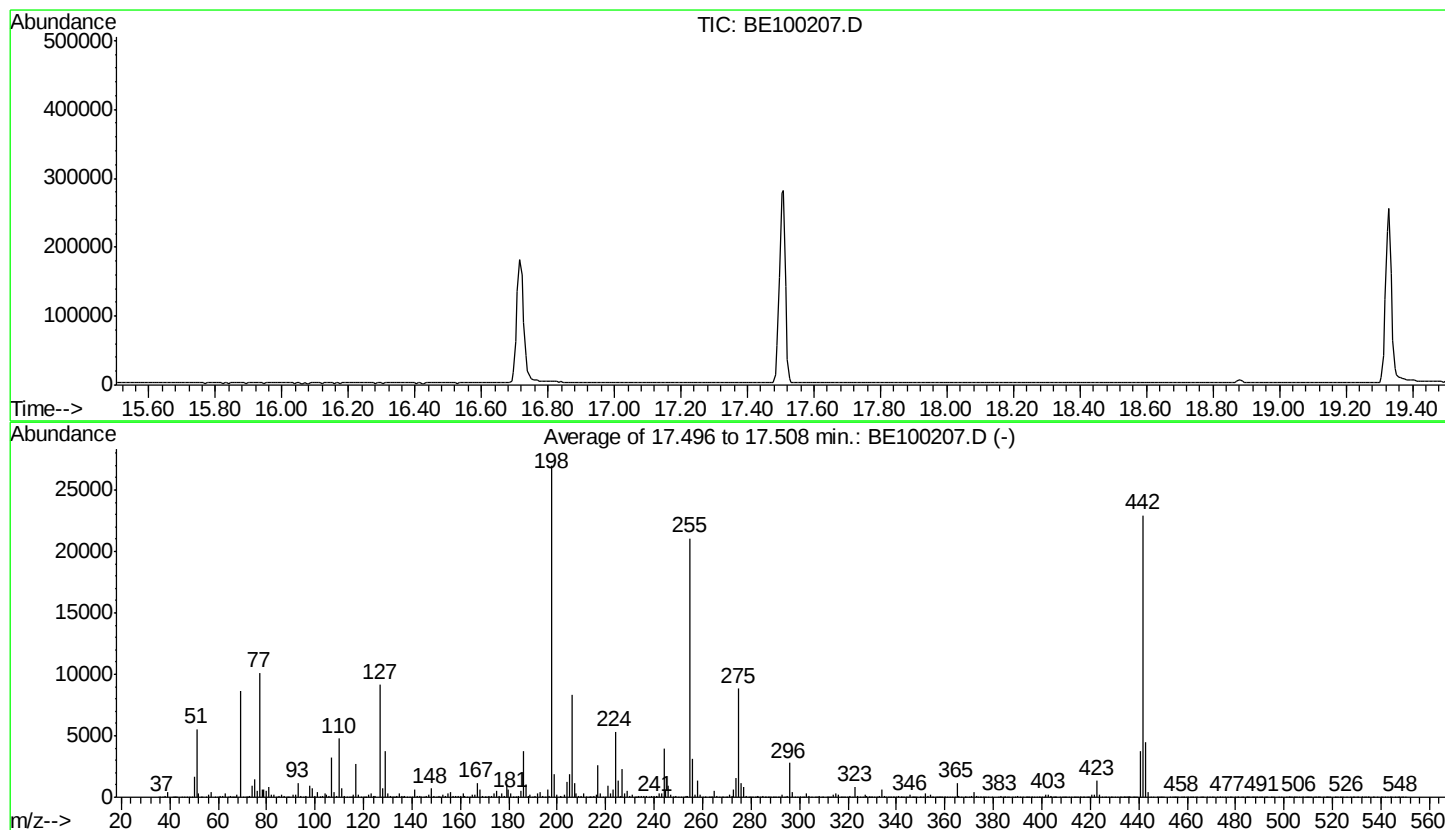

AutoFind: Scans 2537, 2538, 2539; Background Corrected with Scan 2531

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.5	5535	PASS
68	69	0.00	2	1.9	164	PASS
69	198	0.00	100	31.9	8614	PASS
70	69	0.00	2	0.4	33	PASS
127	198	10	80	33.8	9120	PASS
197	198	0.00	2	0.2	61	PASS
198	198	100	100	100.0	26974	PASS
199	198	5	9	6.9	1873	PASS
275	198	10	60	32.8	8849	PASS
365	198	1	100	4.4	1183	PASS
441	198	0.01	100	13.8	3727	PASS
442	198	50	100	85.0	22941	PASS
443	442	15	24	19.4	4444	PASS