


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE062915\
Data File : BE089980.D
Acq On : 29 Jun 2015 12:43
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BE062915.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 30 07:01:01 2015

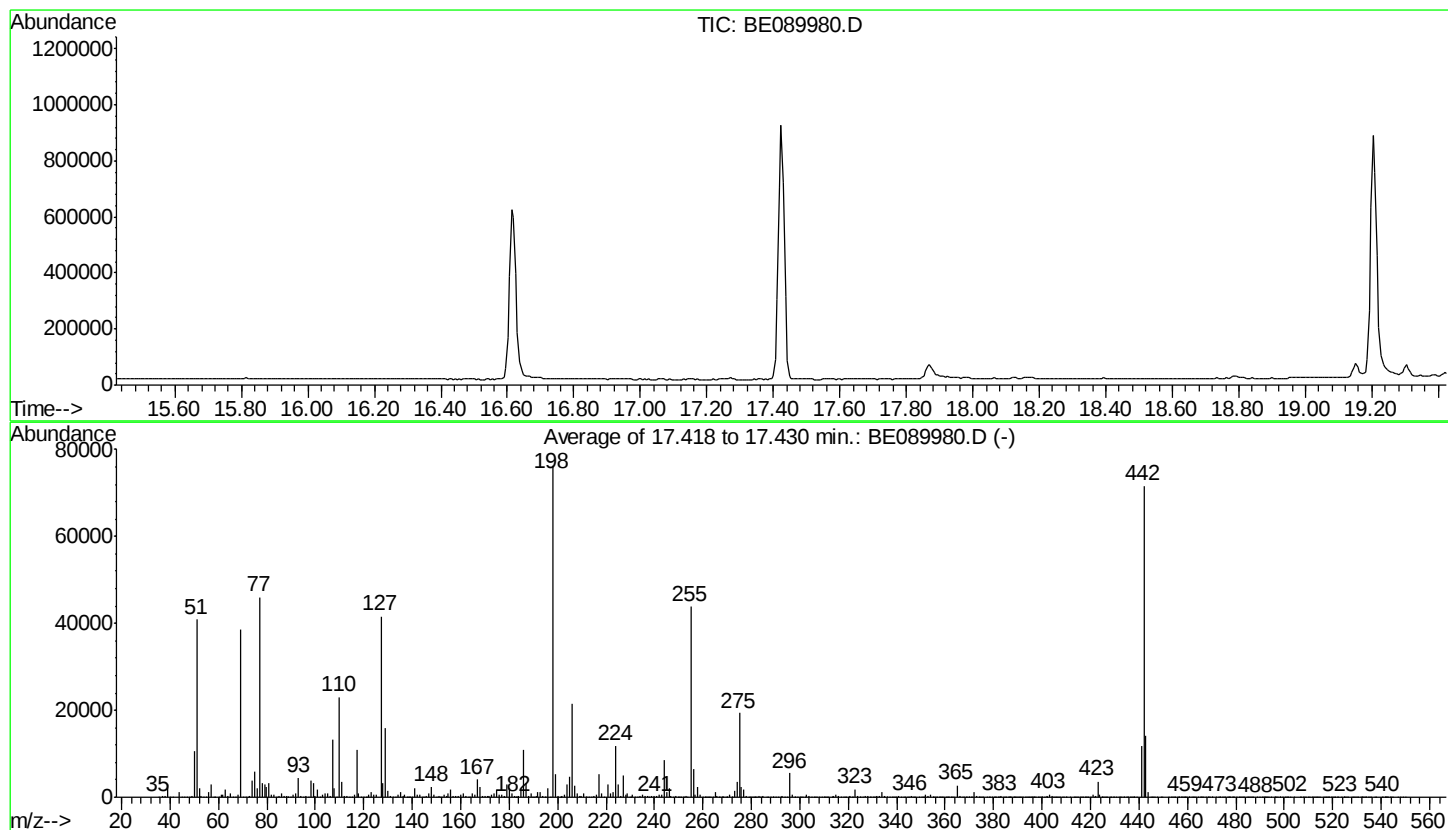

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2516

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.5	40823	PASS
68	69	0.00	2	1.6	637	PASS
69	198	0.00	100	50.6	38631	PASS
70	69	0.00	2	0.3	106	PASS
127	198	10	80	54.5	41596	PASS
197	198	0.00	2	0.2	152	PASS
198	198	100	100	100.0	76301	PASS
199	198	5	9	7.0	5334	PASS
275	198	10	60	25.3	19312	PASS
365	198	1	100	3.6	2740	PASS
441	442	0.01	24	16.6	11882	PASS
442	198	50	100	93.8	71605	PASS
443	442	15	24	19.7	14078	PASS