


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE062915\
 Data File : BE089996.D
 Acq On : 30 Jun 2015 00:33
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BE062915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 30 07:01:01 2015

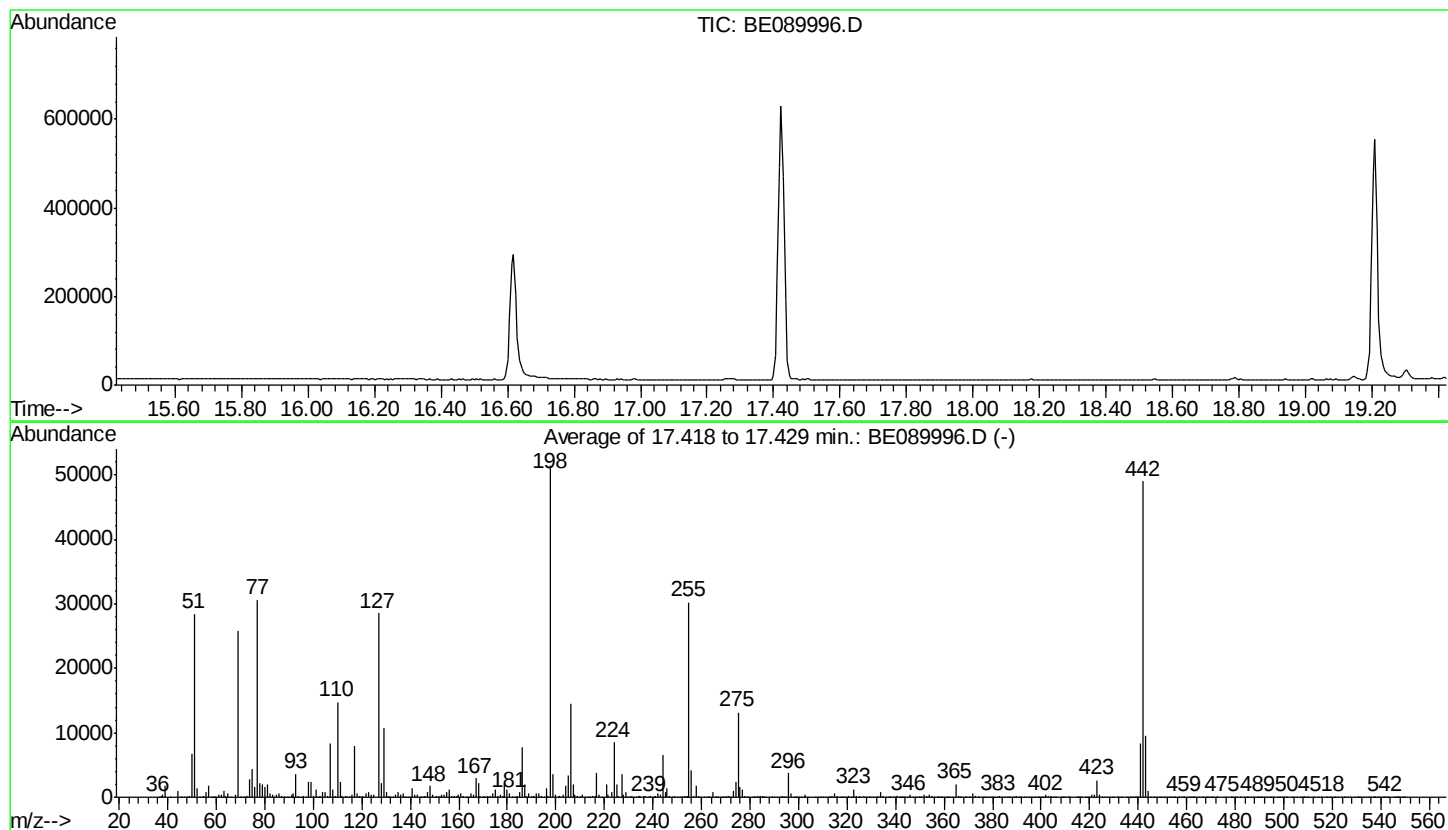

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2517

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.4	28476	PASS
68	69	0.00	2	1.6	420	PASS
69	198	0.00	100	50.1	25781	PASS
70	69	0.00	2	0.4	102	PASS
127	198	10	80	55.6	28574	PASS
197	198	0.00	2	0.4	189	PASS
198	198	100	100	100.0	51424	PASS
199	198	5	9	6.9	3534	PASS
275	198	10	60	25.6	13150	PASS
365	198	1	100	4.0	2042	PASS
441	442	0.01	24	17.2	8441	PASS
442	198	50	100	95.2	48978	PASS
443	442	15	24	19.7	9628	PASS