

Data Path : Z:\HPCHEM1\BNA\_E\DATA\BE063015\  
 Data File : BE090022.D  
 Acq On : 30 Jun 2015 22:06  
 Operator : TP/IZ  
 Sample : G2810-18  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 X1SB0680204-150625

Quant Time: Jul 01 05:19:15 2015  
 Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\8270-SIM-BE062915.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Jun 30 07:01:01 2015  
 Response via : Initial Calibration


| Internal Standards             | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|--------------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4      | 7.62  | 152  | 12873    | 5.00  | ng    | 0.00     |
| 6) Naphthalene-d8              | 10.37 | 136  | 55541    | 5.00  | ng    | -0.01    |
| 12) Acenaphthene-d10           | 14.23 | 164  | 30455    | 5.00  | ng    | 0.00     |
| 18) Phenanthrene-d10           | 16.96 | 188  | 69698    | 5.00  | ng    | -0.02    |
| 25) Chrysene-d12               | 21.12 | 240  | 84622    | 5.00  | ng    | -0.01    |
| 32) Perylene-d12               | 23.44 | 264  | 82637    | 5.00  | ng    | -0.02    |
| System Monitoring Compounds    |       |      |          |       |       |          |
| 4) 2-Fluorophenol              | 5.24  | 112  | 28426    | 9.61  | ng    | 0.00     |
| 5) Phenol-d6                   | 6.80  | 99   | 41318    | 9.98  | ng    | 0.00     |
| 7) Nitrobenzene-d5             | 8.75  | 82   | 24128    | 5.47  | ng    | 0.00     |
| 13) 2,4,6-Tribromophenol       | 15.73 | 330  | 10668    | 11.95 | ng    | 0.00     |
| 14) 2-Fluorobiphenyl           | 12.85 | 172  | 50446    | 5.51  | ng    | -0.01    |
| 27) Terphenyl-d14              | 19.58 | 244  | 76096    | 5.40  | ng    | -0.01    |
| Target Compounds               |       |      |          |       |       |          |
| 2) 1,4-Dioxane                 | 3.15  | 88   | 44       | 0.02  | ng    | # 15     |
| 3) n-Nitrosodimethylamine      | 3.45  | 42   | 574      | 0.24  | ng    | # 1      |
| 9) Naphthalene                 | 10.42 | 128  | 521      | 0.04  | ng    | # 68     |
| 11) 2-Methylnaphthalene        | 12.04 | 142  | 768      | 0.09  | ng    | 96       |
| 21) Pentachlorophenol          | 16.63 | 266  | 13       | 0.27  | ng    | # 54     |
| 30) Bis(2-ethylhexyl)phthalate | 21.05 | 149  | 1538     | 0.46  | ng    | # 96     |
| 31) Indeno(1,2,3-cd)pyrene     | 25.83 | 276  | 453      | 0.02  | ng    | # 91     |
| 37) Benzo(g,h,i)perylene       | 26.57 | 276  | 418      | 0.02  | ng    | # 25     |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA\_E\DATA\BE063015\  
Data File : BE090022.D  
Acq On : 30 Jun 2015 22:06  
Operator : TP/IZ  
Sample : G2810-18  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
X1SB0680204-150625

Quant Time: Jul 01 05:19:15 2015  
Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\8270-SIM-BE062915.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jun 30 07:01:01 2015  
Response via : Initial Calibration

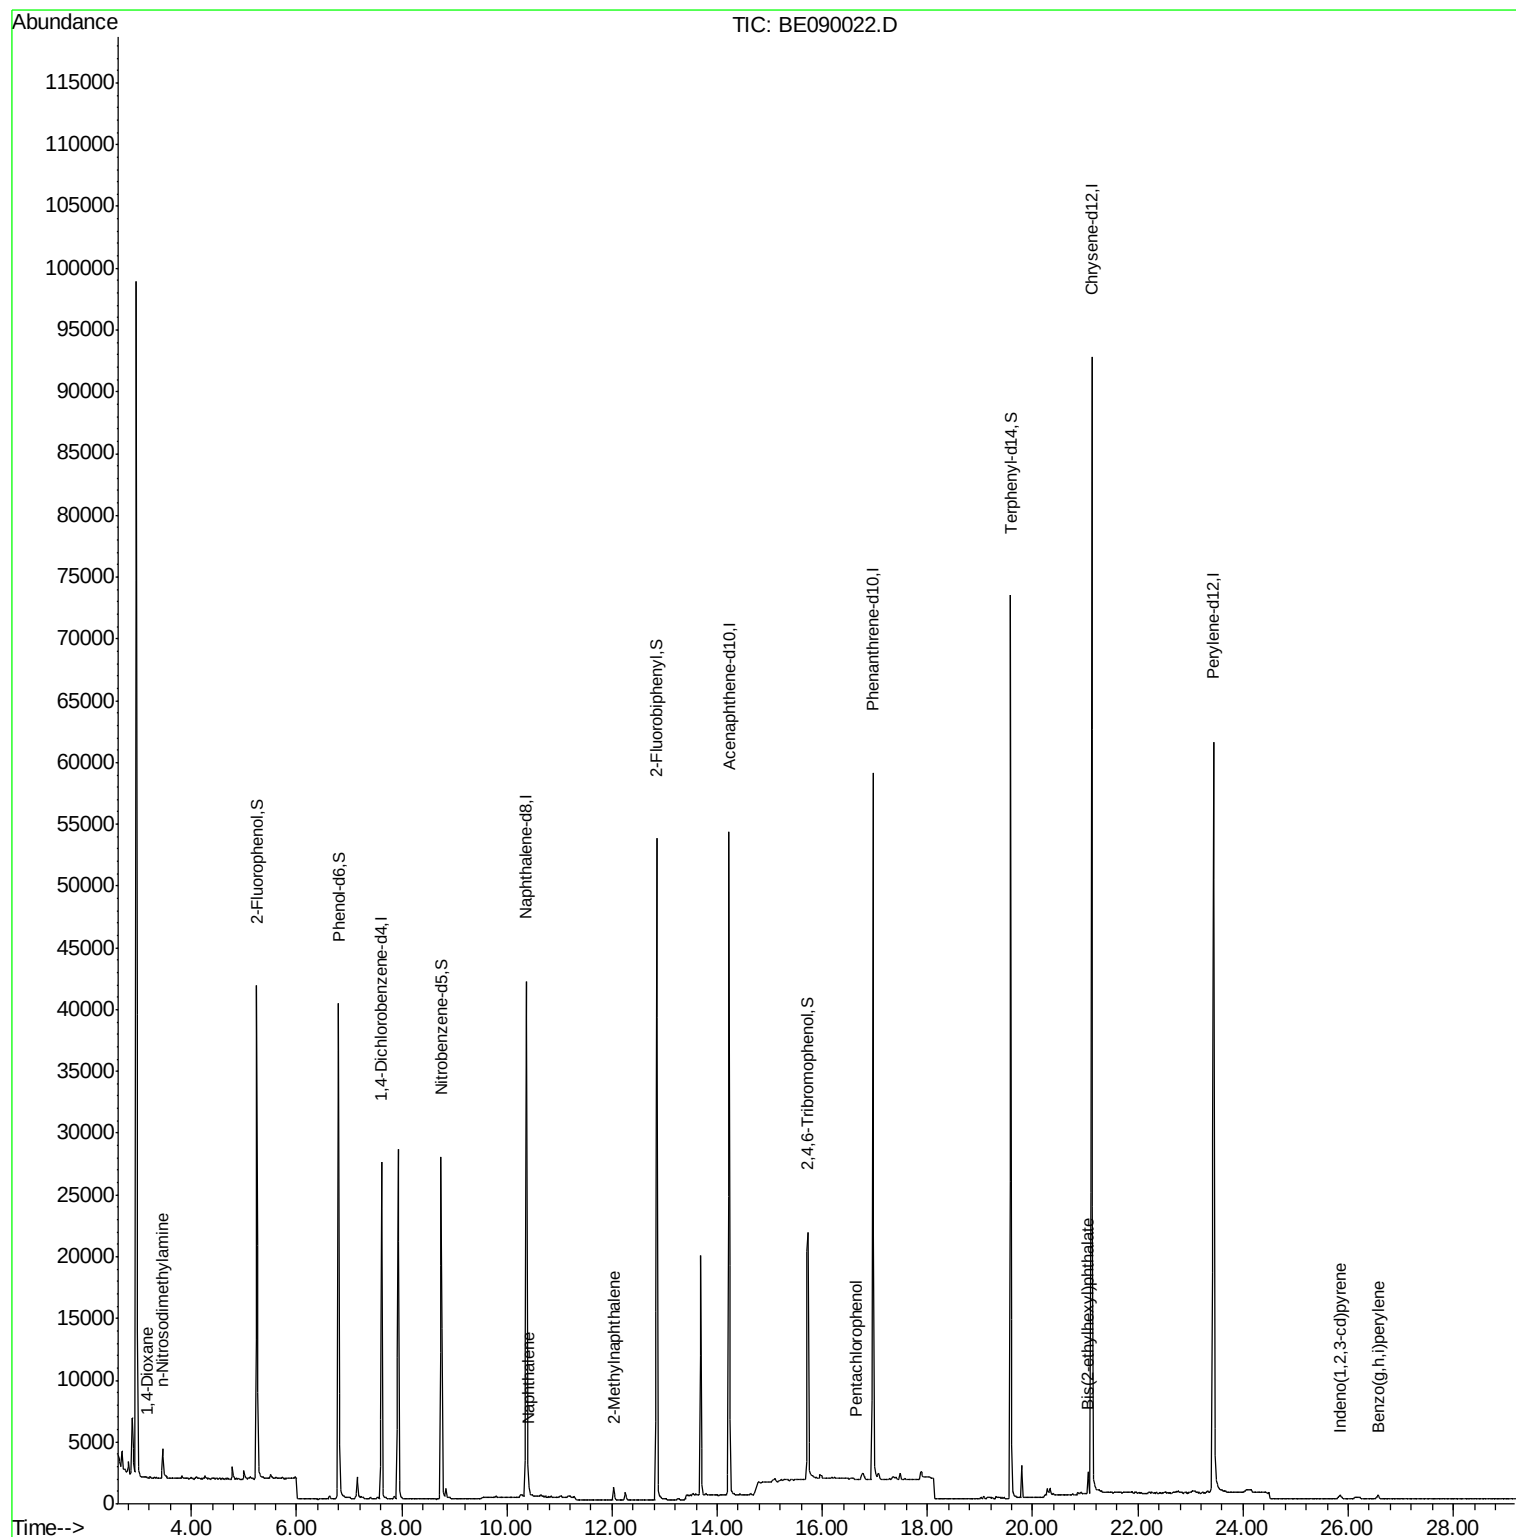




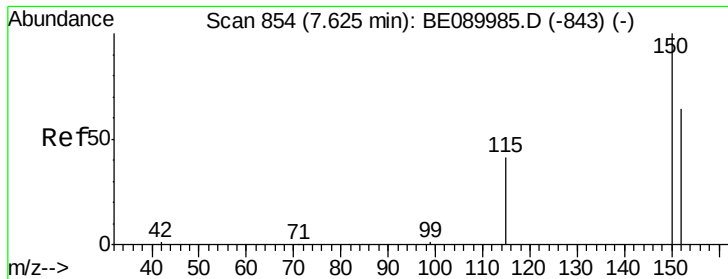


#1

1,4-Dichlorobenzene-d4  
Concen: 5.00 ng  
RT: 7.62 min Scan# 852  
Delta R.T. -0.01 min  
Lab File: BE090022.D  
Acq: 30 Jun 2015 22:06

Instrument :  
BNA\_E  
ClientSampleId :  
X1SB0680204-150625




Tgt Ion: 152 Resp: 12873  
Ion Ratio Lower Upper  
152 100  
150 155.2 123.9 185.9  
115 63.9 50.6 76.0

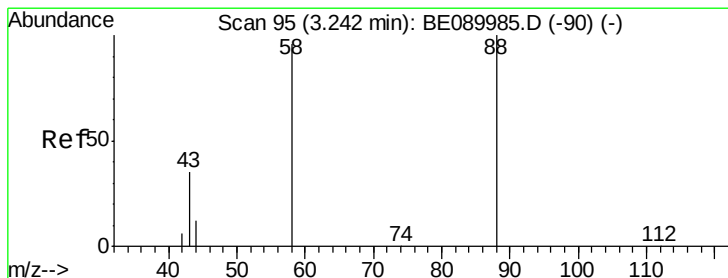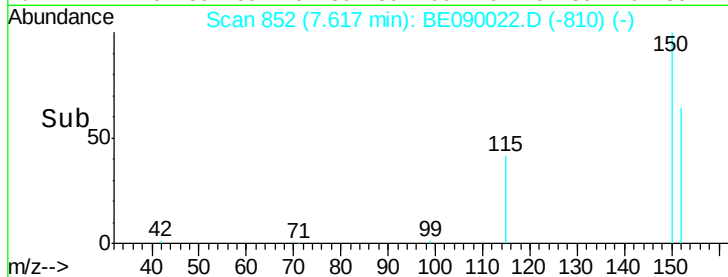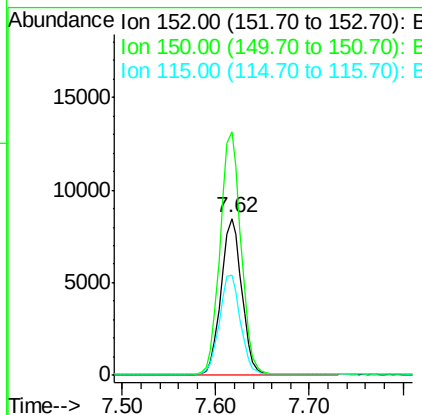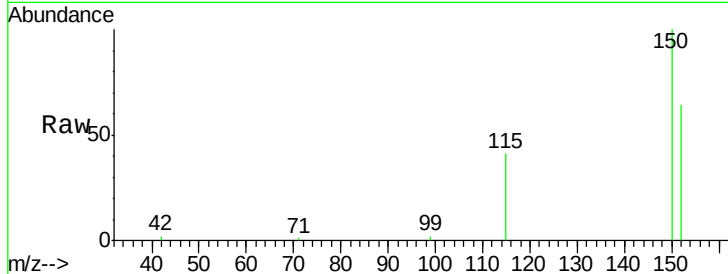


#2

1,4-Dioxane  
Concen: 0.02 ng  
RT: 3.15 min Scan# 82  
Delta R.T. -0.09 min  
Lab File: BE090022.D  
Acq: 30 Jun 2015 22:06

Tgt Ion: 88 Resp: 44  
Ion Ratio Lower Upper  
88 100  
58 0.0 70.9 106.3#  
43 0.0 27.6 41.4#

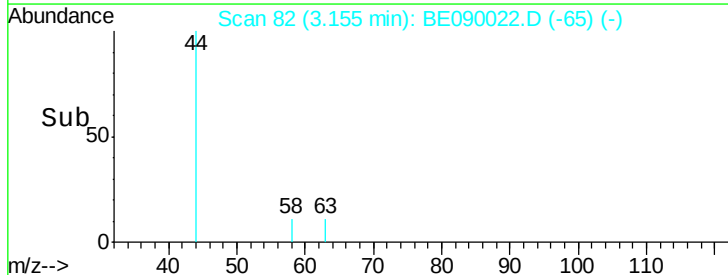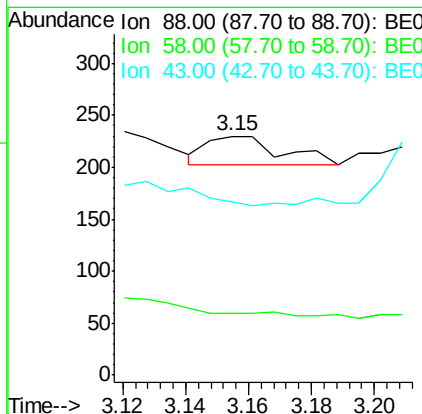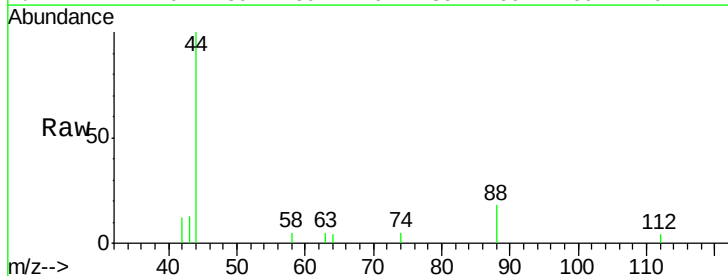

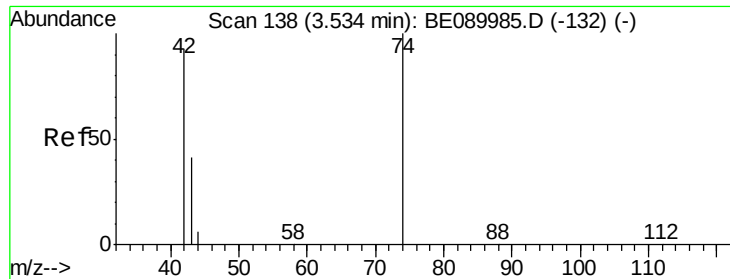

#3

n-Nitrosodimethylamine

Concen: 0.24 ng

RT: 3.45 min Scan# 126

Delta R.T. -0.08 min

Lab File: BE090022.D

Acq: 30 Jun 2015 22:06

Instrument :

BNA\_E

ClientSampleId :

X1SB0680204-150625





Tgt Ion: 42 Resp: 574

Ion Ratio Lower Upper

42 100

74 2.6 89.4 134.2#

44 158.2 6.9 10.3#

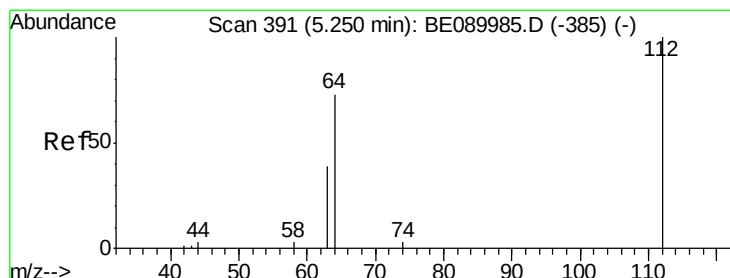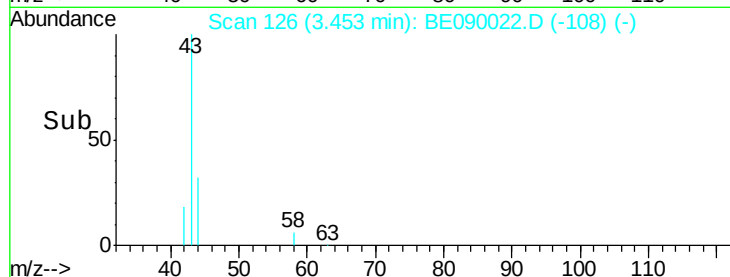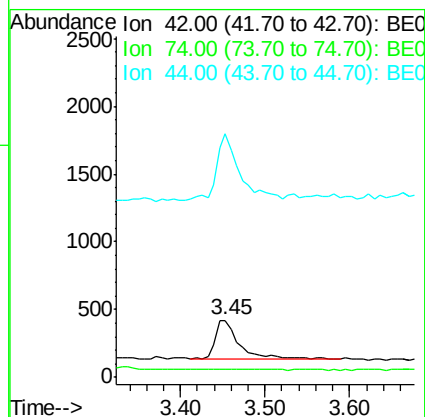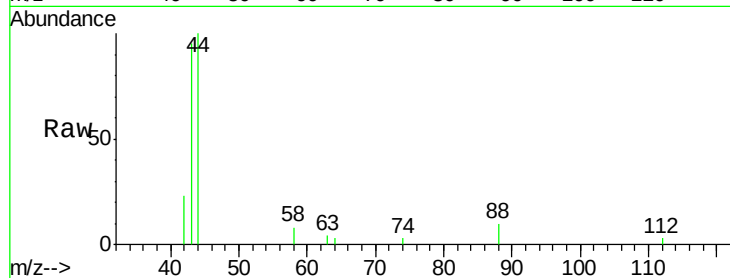

#4

2-Fluorophenol

Concen: 9.61 ng

RT: 5.24 min Scan# 390

Delta R.T. -0.01 min

Lab File: BE090022.D

Acq: 30 Jun 2015 22:06




Tgt Ion: 112 Resp: 28426


Ion Ratio Lower Upper

112 100

64 70.5 56.3 84.5

63 36.4 29.8 44.6

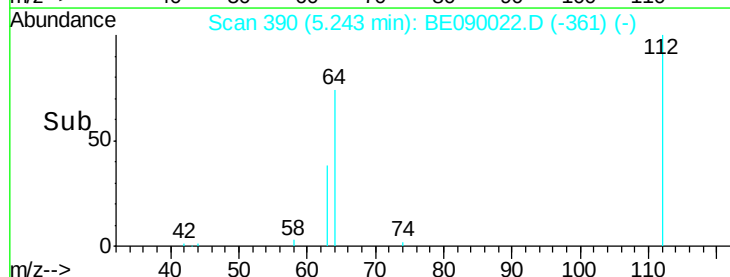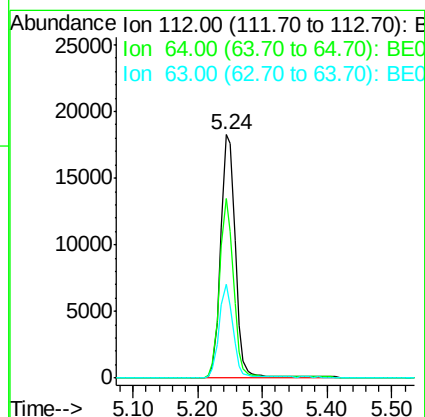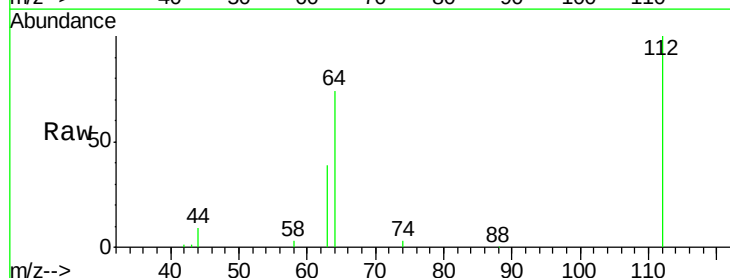

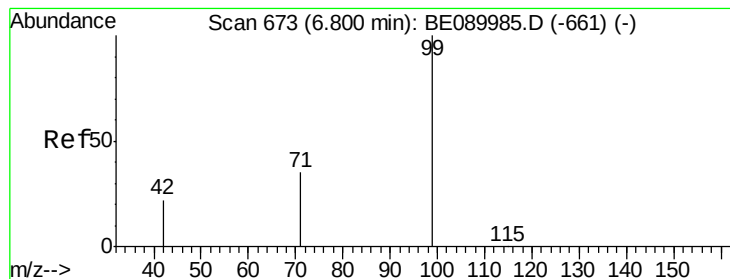

#5

Phenol-d6

Concen: 9.98 ng

RT: 6.80 min Scan# 672

Delta R.T. -0.00 min

Lab File: BE090022.D

Acq: 30 Jun 2015 22:06

Instrument :

BNA\_E

ClientSampleId :

X1SB0680204-150625





Tgt Ion: 99 Resp: 41318

Ion Ratio Lower Upper

99 100

42 20.4 18.7 28.1

71 34.0 27.5 41.3

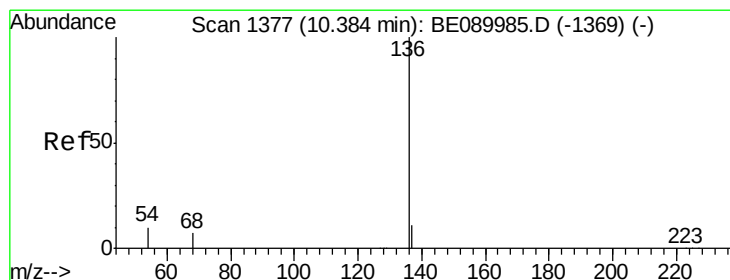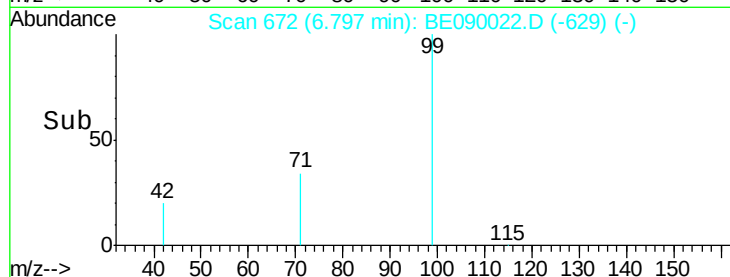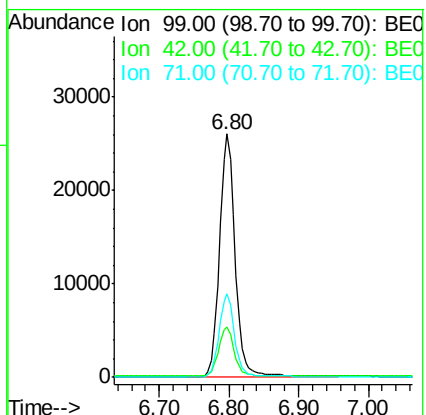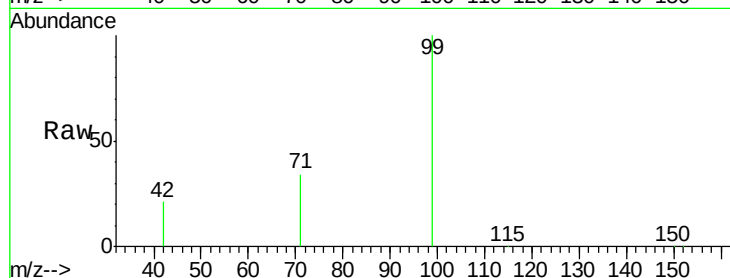

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.37 min Scan# 1375

Delta R.T. -0.01 min

Lab File: BE090022.D

Acq: 30 Jun 2015 22:06

Tgt Ion: 136 Resp: 55541




Ion Ratio Lower Upper


136 100

137 10.9 8.9 13.3

54 12.1 8.2 12.4

68 8.7 5.8 8.8

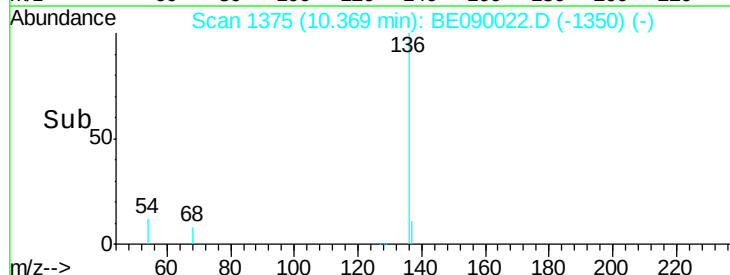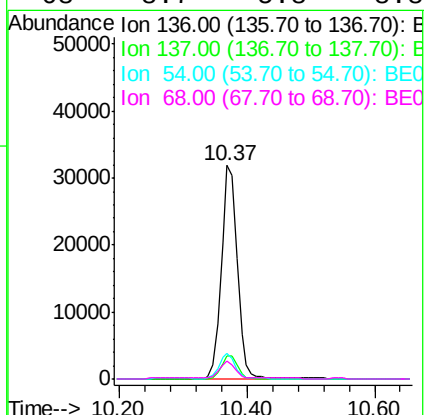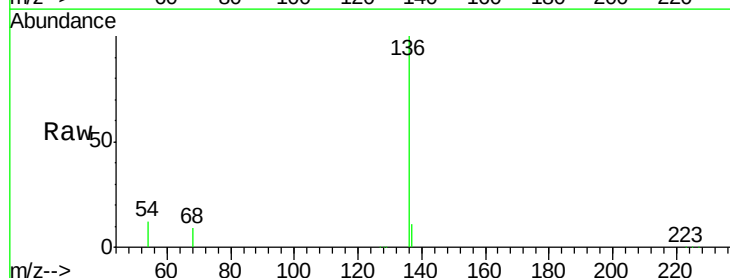

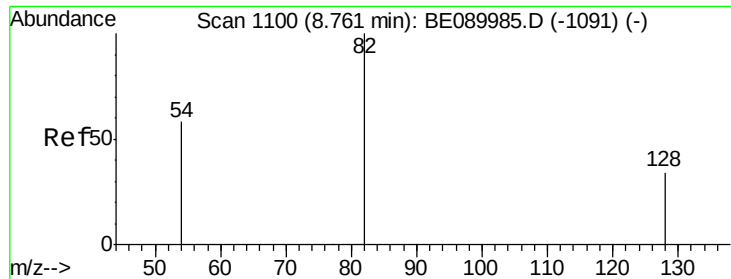

#7

Nitrobenzene-d5

Concen: 5.47 ng

RT: 8.75 min Scan# 1098

Delta R.T. -0.01 min

Lab File: BE090022.D

Acq: 30 Jun 2015 22:06

Instrument :

BNA\_E

ClientSampleId :

X1SB0680204-150625





Tgt Ion: 82 Resp: 24128

Ion Ratio Lower Upper

82 100

128 35.5 28.0 42.0

54 59.0 47.6 71.4

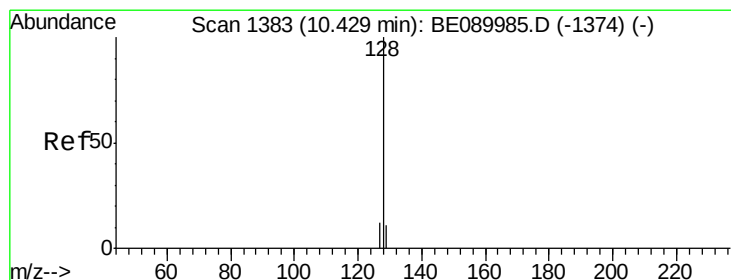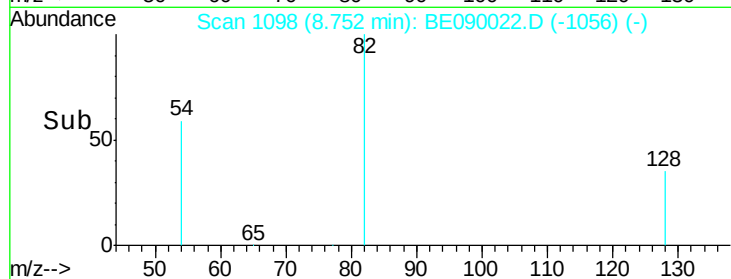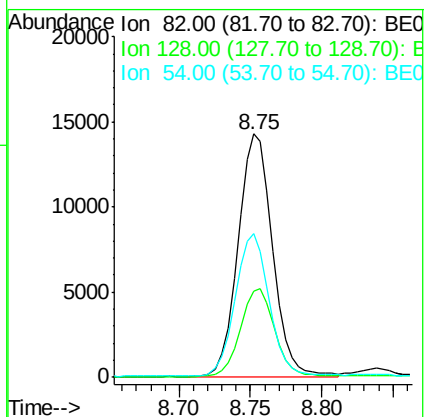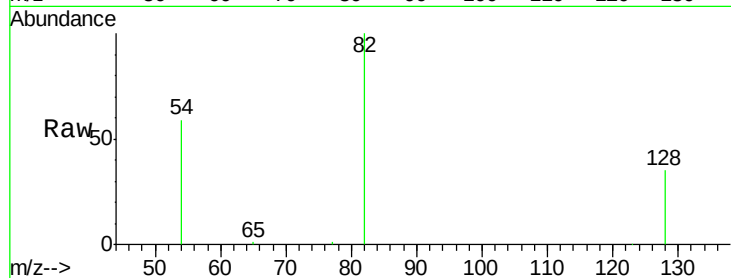

#9

Naphthalene

Concen: 0.04 ng

RT: 10.42 min Scan# 1382

Delta R.T. -0.01 min

Lab File: BE090022.D

Acq: 30 Jun 2015 22:06




Tgt Ion: 128 Resp: 521


Ion Ratio Lower Upper

128 100

129 25.1 9.3 13.9#

127 24.5 10.2 15.4#


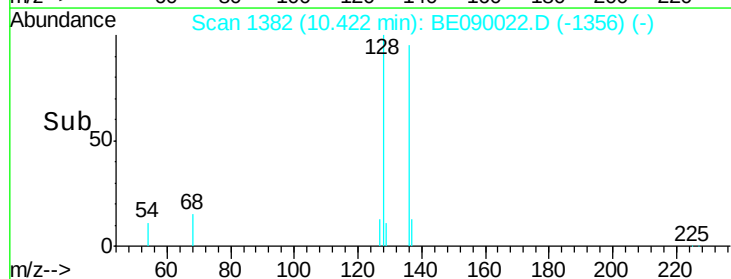
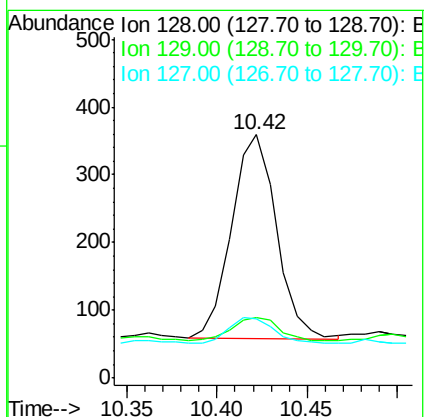
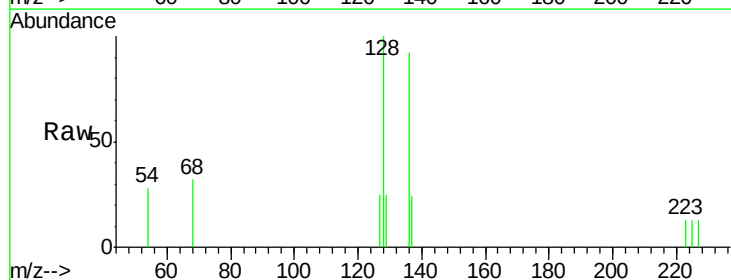


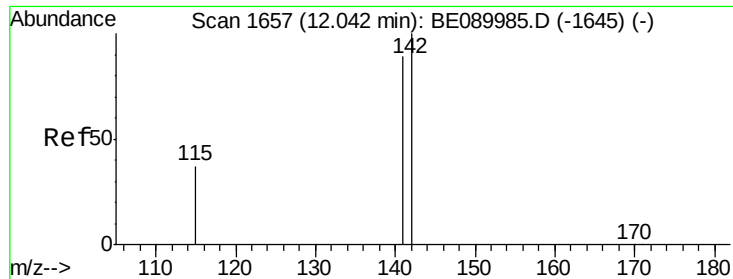

#11  
2-Methylnaphthalene  
Concen: 0.09 ng  
RT: 12.04 min Scan# 1656  
Delta R.T. -0.01 min  
Lab File: BE090022.D  
Acq: 30 Jun 2015 22:06




Instrument :  
BNA\_E  
ClientSampleId :  
X1SB0680204-150625


Tgt Ion:142 Resp: 768  
Ion Ratio Lower Upper  
142 100  
141 87.7 71.3 106.9  
115 43.9 30.4 45.6

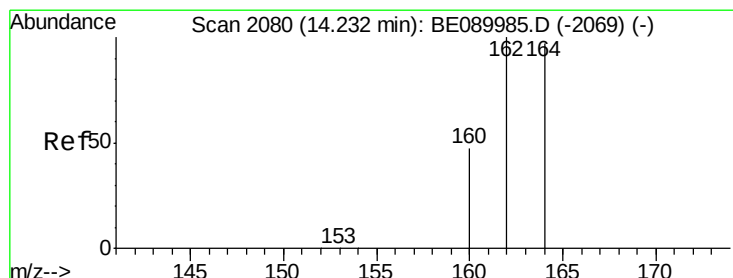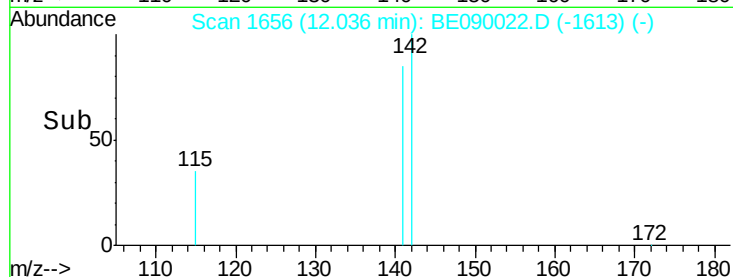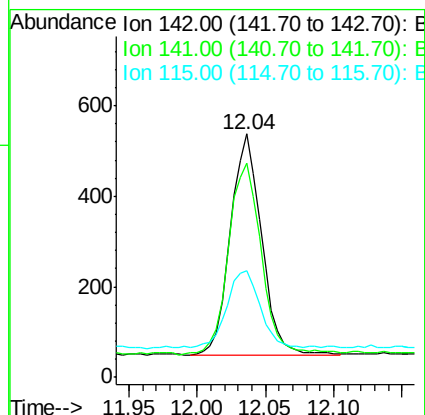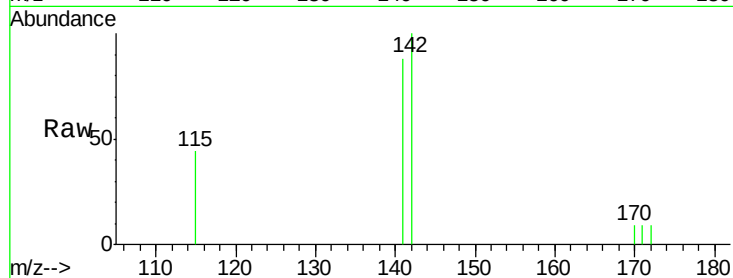

#12  
Acenaphthene-d10  
Concen: 5.00 ng  
RT: 14.23 min Scan# 2079  
Delta R.T. -0.01 min  
Lab File: BE090022.D  
Acq: 30 Jun 2015 22:06

Tgt Ion:164 Resp: 30455  
Ion Ratio Lower Upper  
164 100  
162 104.6 82.2 123.4  
160 48.1 39.0 58.6

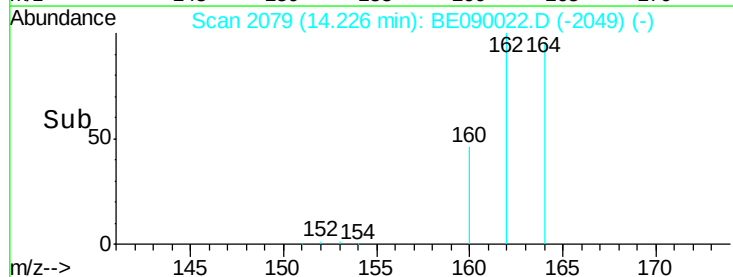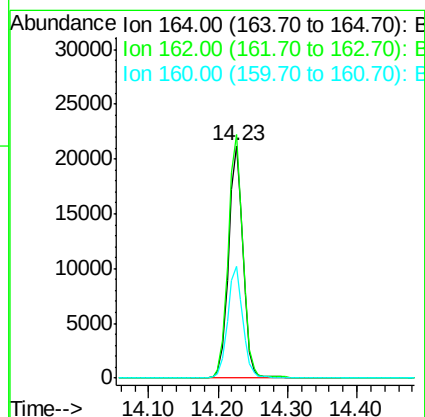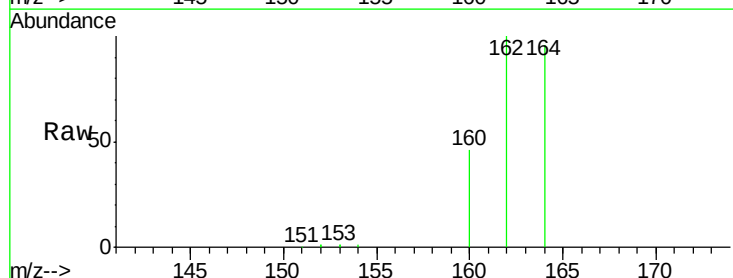


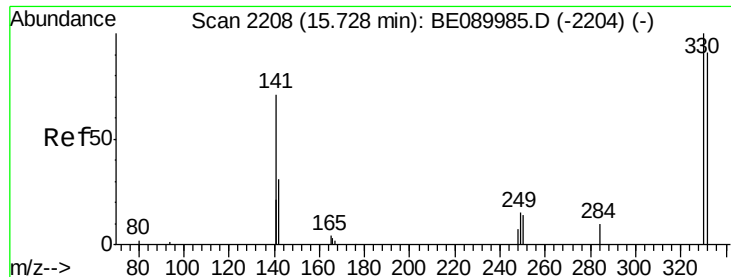




#13  
 2,4,6-Tribromophenol  
 Concen: 11.95 ng  
 RT: 15.73 min Scan# 2207  
 Delta R.T. -0.00 min  
 Lab File: BE090022.D  
 Acq: 30 Jun 2015 22:06

Instrument :  
 BNA\_E  
 ClientSampleId :  
 X1SB0680204-150625

Tgt Ion:330 Resp: 10668  
 Ion Ratio Lower Upper  
 330 100  
 332 97.0 76.4 114.6  
 141 164.2 130.3 195.5

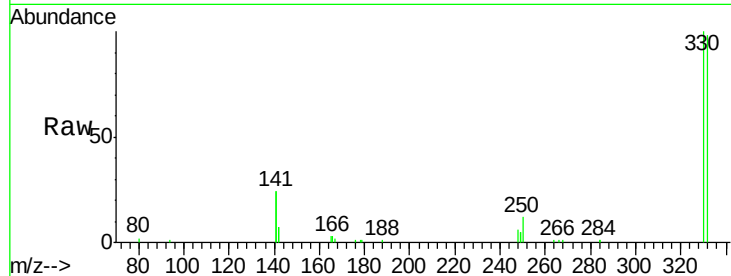


Abundance Ion 329.80 (329.50 to 330.50): E  
 Ion 331.80 (331.50 to 332.50): E  
 Ion 141.00 (140.70 to 141.70): E

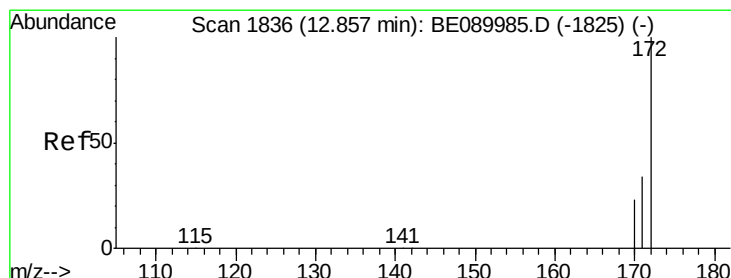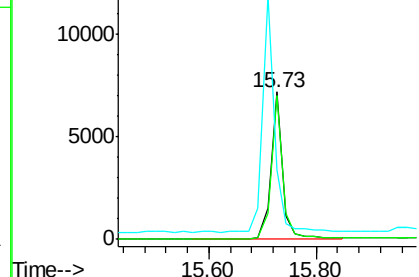
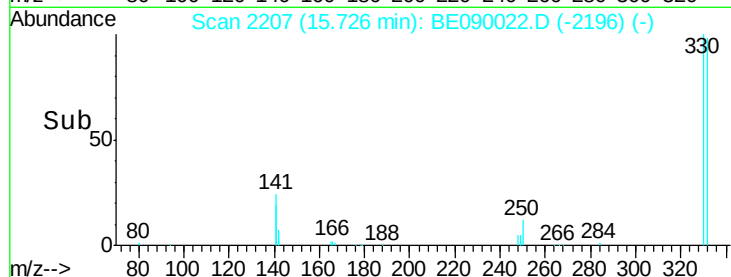


#14  
 2-Fluorobiphenyl  
 Concen: 5.51 ng  
 RT: 12.85 min Scan# 1834  
 Delta R.T. -0.01 min  
 Lab File: BE090022.D  
 Acq: 30 Jun 2015 22:06


Tgt Ion:172 Resp: 50446  
 Ion Ratio Lower Upper  
 172 100  
 171 35.9 27.8 41.6  
 170 24.2 18.3 27.5

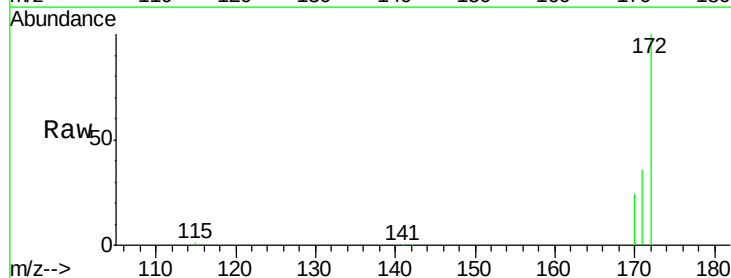

Abundance Ion 172.00 (171.70 to 172.70): E  
 Ion 171.00 (170.70 to 171.70): E  
 Ion 170.00 (169.70 to 170.70): E

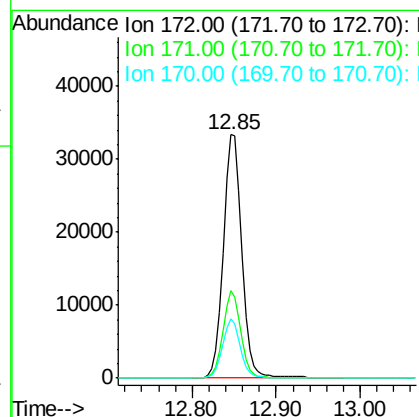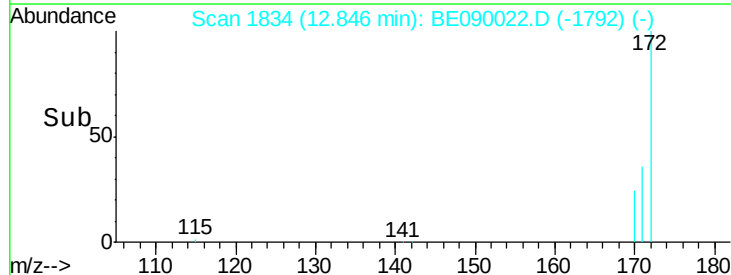



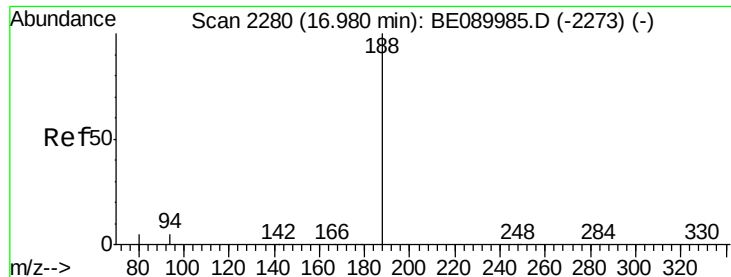

#18

Phenanthrene-d10

Concen: 5.00 ng

RT: 16.96 min Scan# 2278

Delta R.T. -0.02 min

Lab File: BE090022.D

Acq: 30 Jun 2015 22:06

Instrument :

BNA\_E

ClientSampleId :

X1SB0680204-150625


Tgt Ion:188 Resp: 69698

Ion Ratio Lower Upper

188 100

94 13.1 4.1 6.1#




80 14.6 4.2 6.2#

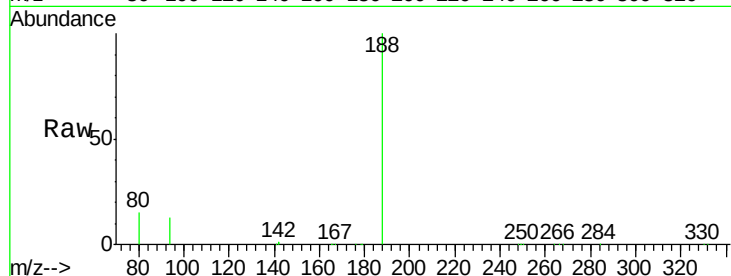

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

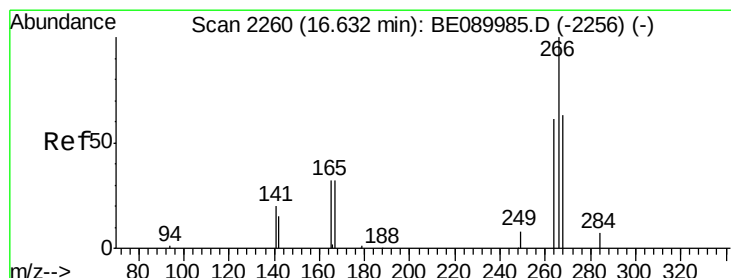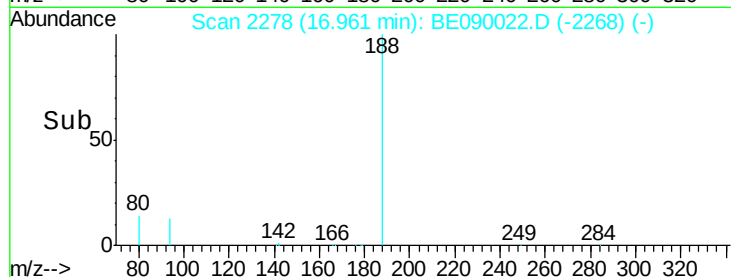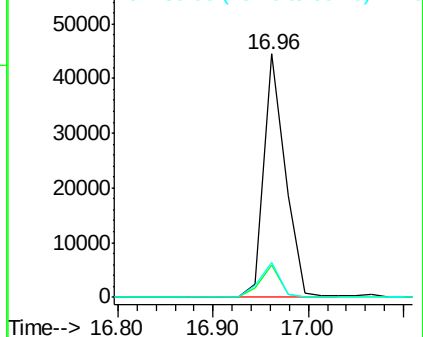

#21

Pentachlorophenol

Concen: 0.27 ng

RT: 16.63 min Scan# 2259

Delta R.T. -0.00 min

Lab File: BE090022.D

Acq: 30 Jun 2015 22:06


Tgt Ion:266 Resp: 13

Ion Ratio Lower Upper

266 100

268 102.0 51.8 77.8#



264 98.0 50.2 75.2#

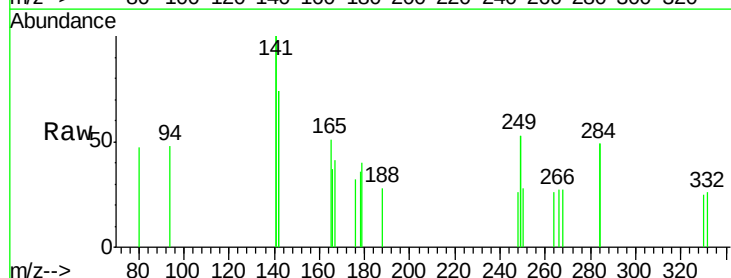


Abundance Ion 265.70 (265.40 to 266.40): E

Ion 268.00 (267.70 to 268.70): E

Ion 264.00 (263.70 to 264.70): E



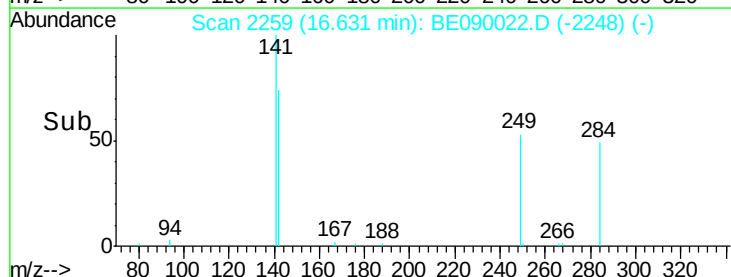
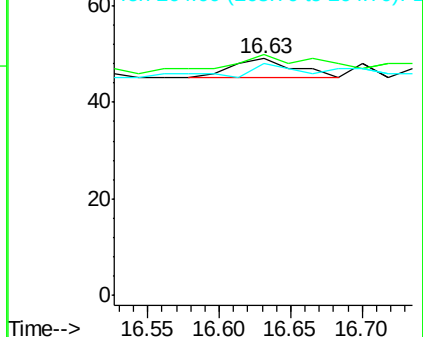


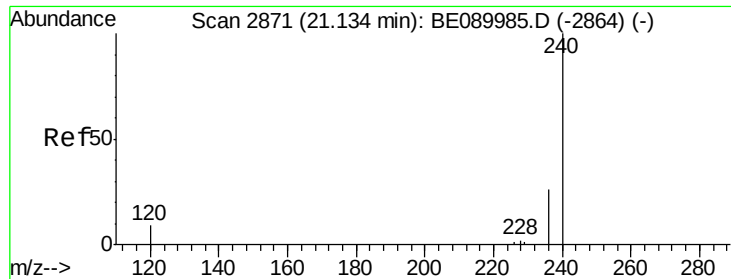

#25  
Chrysene-d12  
Concen: 5.00 ng  
RT: 21.12 min Scan# 2868  
Delta R.T. -0.01 min  
Lab File: BE090022.D  
Acq: 30 Jun 2015 22:06




Instrument :  
BNA\_E  
ClientSampleId :  
X1SB0680204-150625


Tgt Ion:240 Resp: 84622  
Ion Ratio Lower Upper  
240 100  
120 10.9 6.9 10.3#  
236 26.5 20.8 31.2

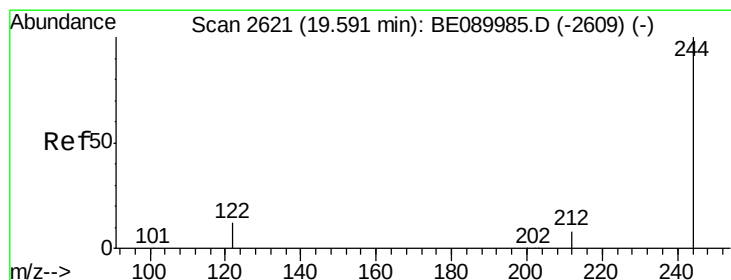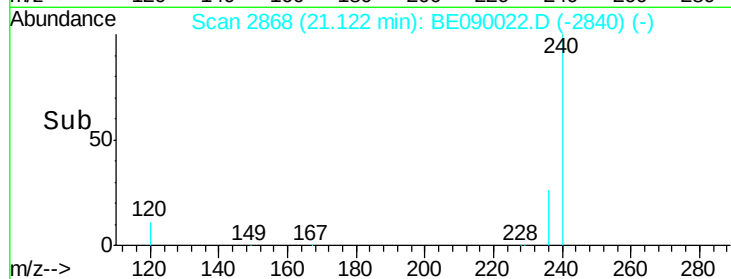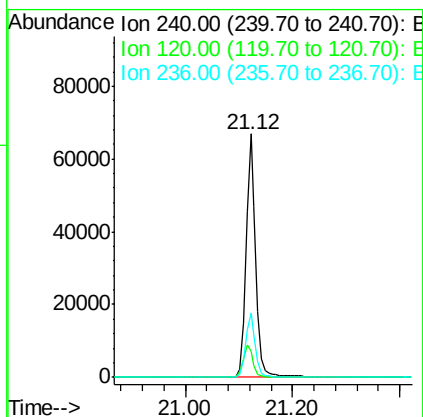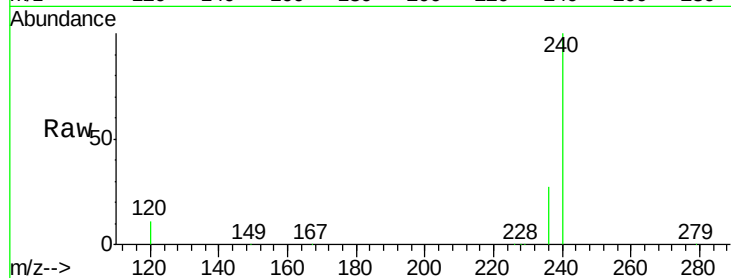

#27  
Terphenyl-d14  
Concen: 5.40 ng  
RT: 19.58 min Scan# 2618  
Delta R.T. -0.01 min  
Lab File: BE090022.D  
Acq: 30 Jun 2015 22:06

Tgt Ion:244 Resp: 76096  
Ion Ratio Lower Upper  
244 100  
212 8.0 6.6 9.8  
122 13.8 9.8 14.8

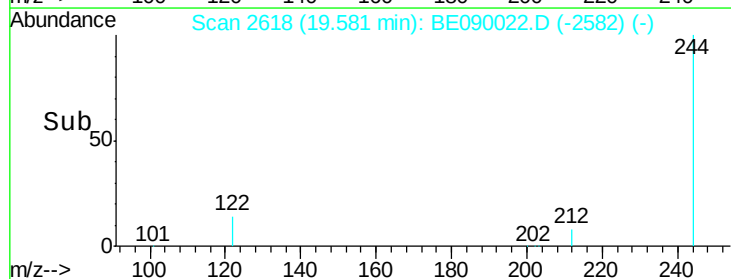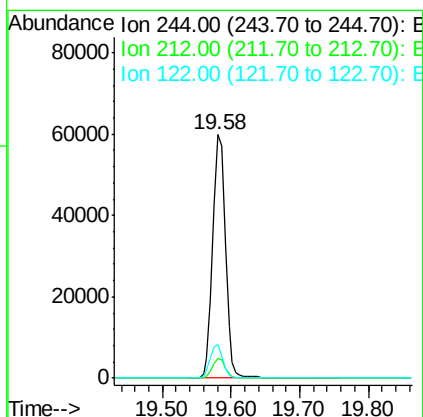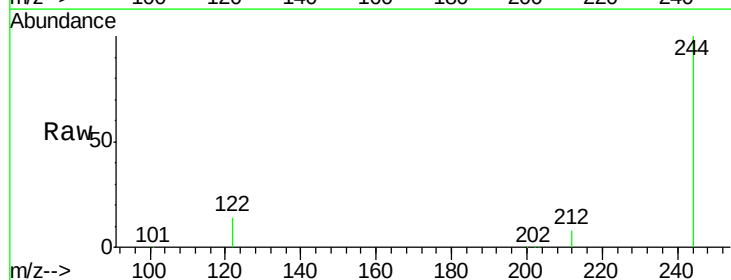

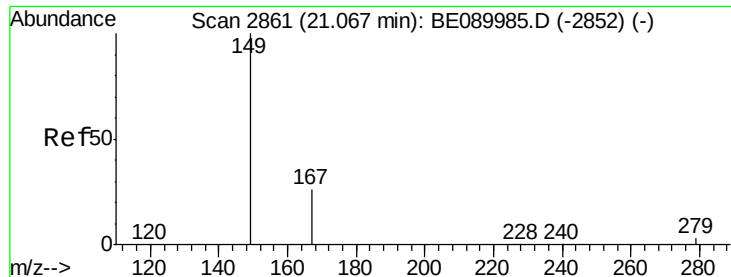

#30

Bis(2-ethylhexyl)phthalate

Concen: 0.46 ng

RT: 21.05 min Scan# 2858

Delta R.T. -0.01 min

Lab File: BE090022.D

Acq: 30 Jun 2015 22:06

Instrument :

BNA\_E

ClientSampleId :

X1SB0680204-150625


Tgt Ion:149 Resp: 1538

Ion Ratio Lower Upper

149 100

167 27.5 20.3 30.5




279 4.0 2.6 3.8#

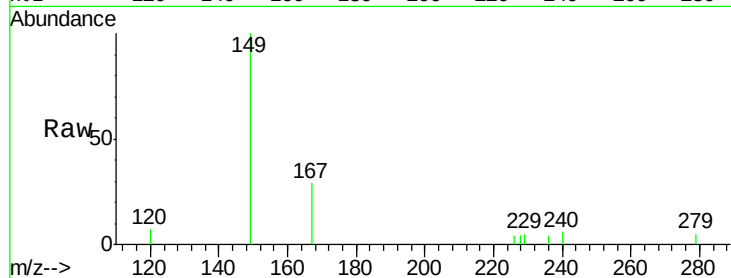

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

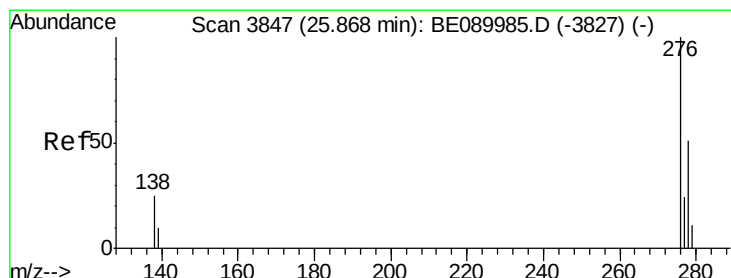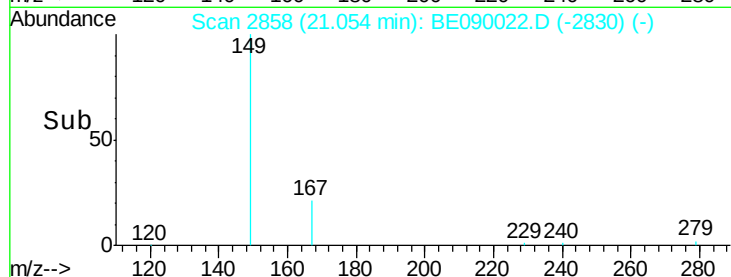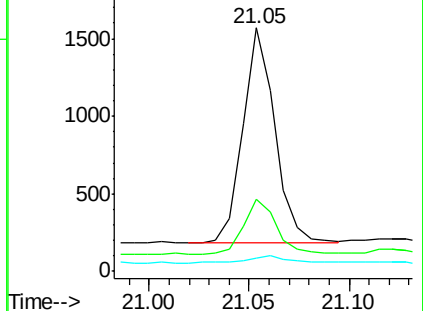

#31

Indeno(1,2,3-cd)pyrene

Concen: 0.02 ng

RT: 25.83 min Scan# 3838

Delta R.T. -0.04 min

Lab File: BE090022.D

Acq: 30 Jun 2015 22:06


Tgt Ion:276 Resp: 453

Ion Ratio Lower Upper

276 100

138 19.2 21.3 31.9#



277 26.3 19.7 29.5

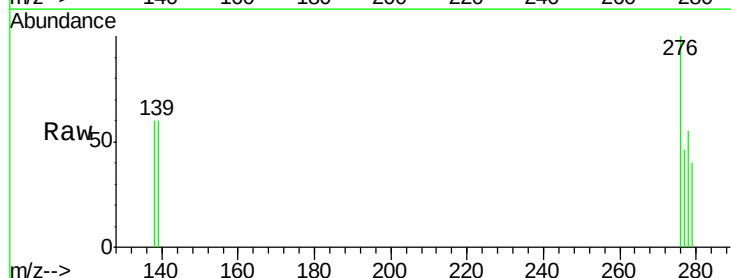


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

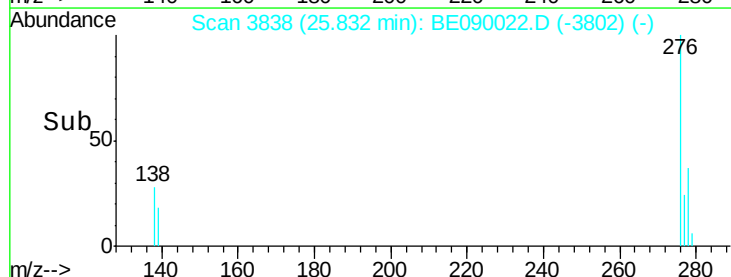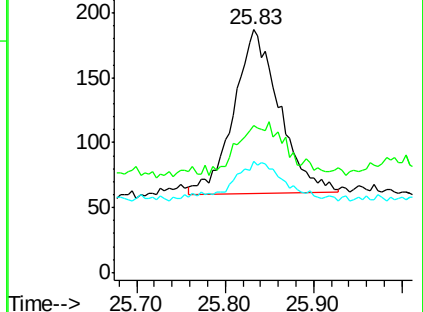

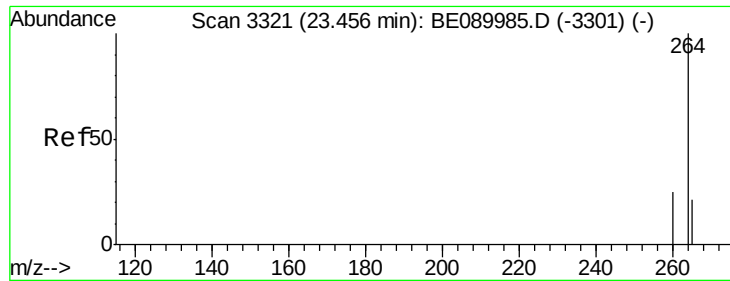

#32

Perylene-d12

Concen: 5.00 ng

RT: 23.44 min Scan# 3316

Delta R.T. -0.02 min

Lab File: BE090022.D

Acq: 30 Jun 2015 22:06

Instrument :

BNA\_E

ClientSampleId :

X1SB0680204-150625


Tgt Ion:264 Resp: 82637

Ion Ratio Lower Upper

264 100

260 24.9 20.2 30.2




265 22.1 17.1 25.7

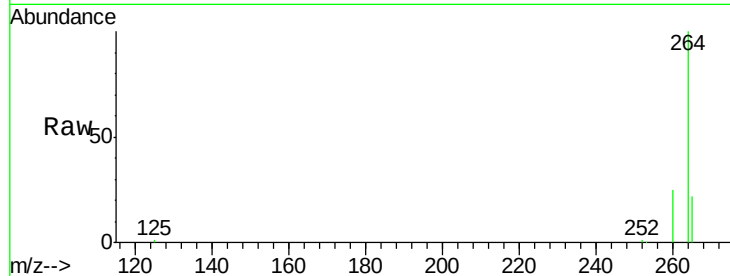

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

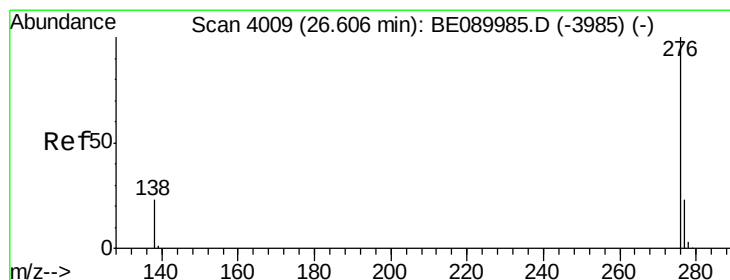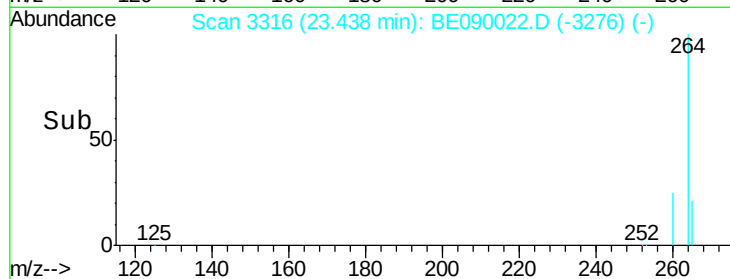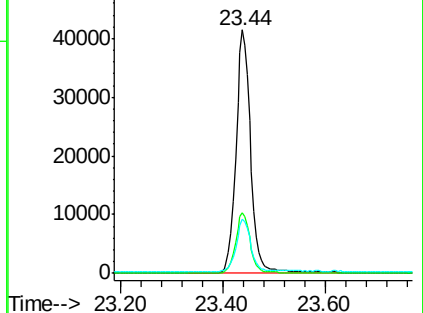

#37

Benzo(g,h,i)perylene

Concen: 0.02 ng

RT: 26.57 min Scan# 3999

Delta R.T. -0.04 min

Lab File: BE090022.D

Acq: 30 Jun 2015 22:06


Tgt Ion:276 Resp: 418

Ion Ratio Lower Upper

276 100

277 49.1 18.8 28.2#

138 71.1 18.6 27.8#

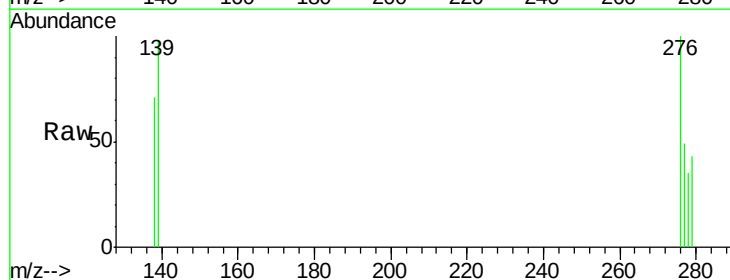

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

