

Data Path : Z:\HPCHEM1\BNA\_E\DATA\BE063015\  
 Data File : BE090026.D  
 Acq On : 1 Jul 2015 00:32  
 Operator : TP/IZ  
 Sample : G2811-04  
 Misc :  
 ALS Vial : 15 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 X1SB0520204-150625

Quant Time: Jul 01 06:12:45 2015  
 Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\8270-SIM-BE062915.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Jun 30 07:01:01 2015  
 Response via : Initial Calibration


| Internal Standards             | R.T.  | QIon | Response | Conc | Units | Dev(Min)       |
|--------------------------------|-------|------|----------|------|-------|----------------|
| 1) 1,4-Dichlorobenzene-d4      | 7.62  | 152  | 14266    | 5.00 | ng    | 0.00           |
| 6) Naphthalene-d8              | 10.37 | 136  | 61936    | 5.00 | ng    | -0.01          |
| 12) Acenaphthene-d10           | 14.22 | 164  | 34435    | 5.00 | ng    | 0.00           |
| 18) Phenanthrene-d10           | 16.96 | 188  | 77640    | 5.00 | ng    | -0.02          |
| 25) Chrysene-d12               | 21.12 | 240  | 93223    | 5.00 | ng    | -0.01          |
| 32) Perylene-d12               | 23.44 | 264  | 90293    | 5.00 | ng    | -0.02          |
| System Monitoring Compounds    |       |      |          |      |       |                |
| 4) 2-Fluorophenol              | 5.24  | 112  | 17911    | 5.47 | ng    | 0.00           |
| 5) Phenol-d6                   | 6.80  | 99   | 26141    | 5.70 | ng    | 0.00           |
| 7) Nitrobenzene-d5             | 8.75  | 82   | 15173    | 3.08 | ng    | 0.00           |
| 13) 2,4,6-Tribromophenol       | 15.73 | 330  | 6321     | 6.26 | ng    | 0.00           |
| 14) 2-Fluorobiphenyl           | 12.85 | 172  | 32318    | 3.12 | ng    | 0.00           |
| 27) Terphenyl-d14              | 19.58 | 244  | 46851    | 3.02 | ng    | -0.01          |
| Target Compounds               |       |      |          |      |       |                |
| 30) Bis(2-ethylhexyl)phthalate | 21.05 | 149  | 1031     | 0.40 | ng    | Qvalue<br># 93 |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA\_E\DATA\BE063015\  
Data File : BE090026.D  
Acq On : 1 Jul 2015 00:32  
Operator : TP/IZ  
Sample : G2811-04  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
X1SB0520204-150625

Quant Time: Jul 01 06:12:45 2015  
Quant Method : Z:\HPCHEM1\BNA\_M\METHODS\8270-SIM-BE062915.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jun 30 07:01:01 2015  
Response via : Initial Calibration

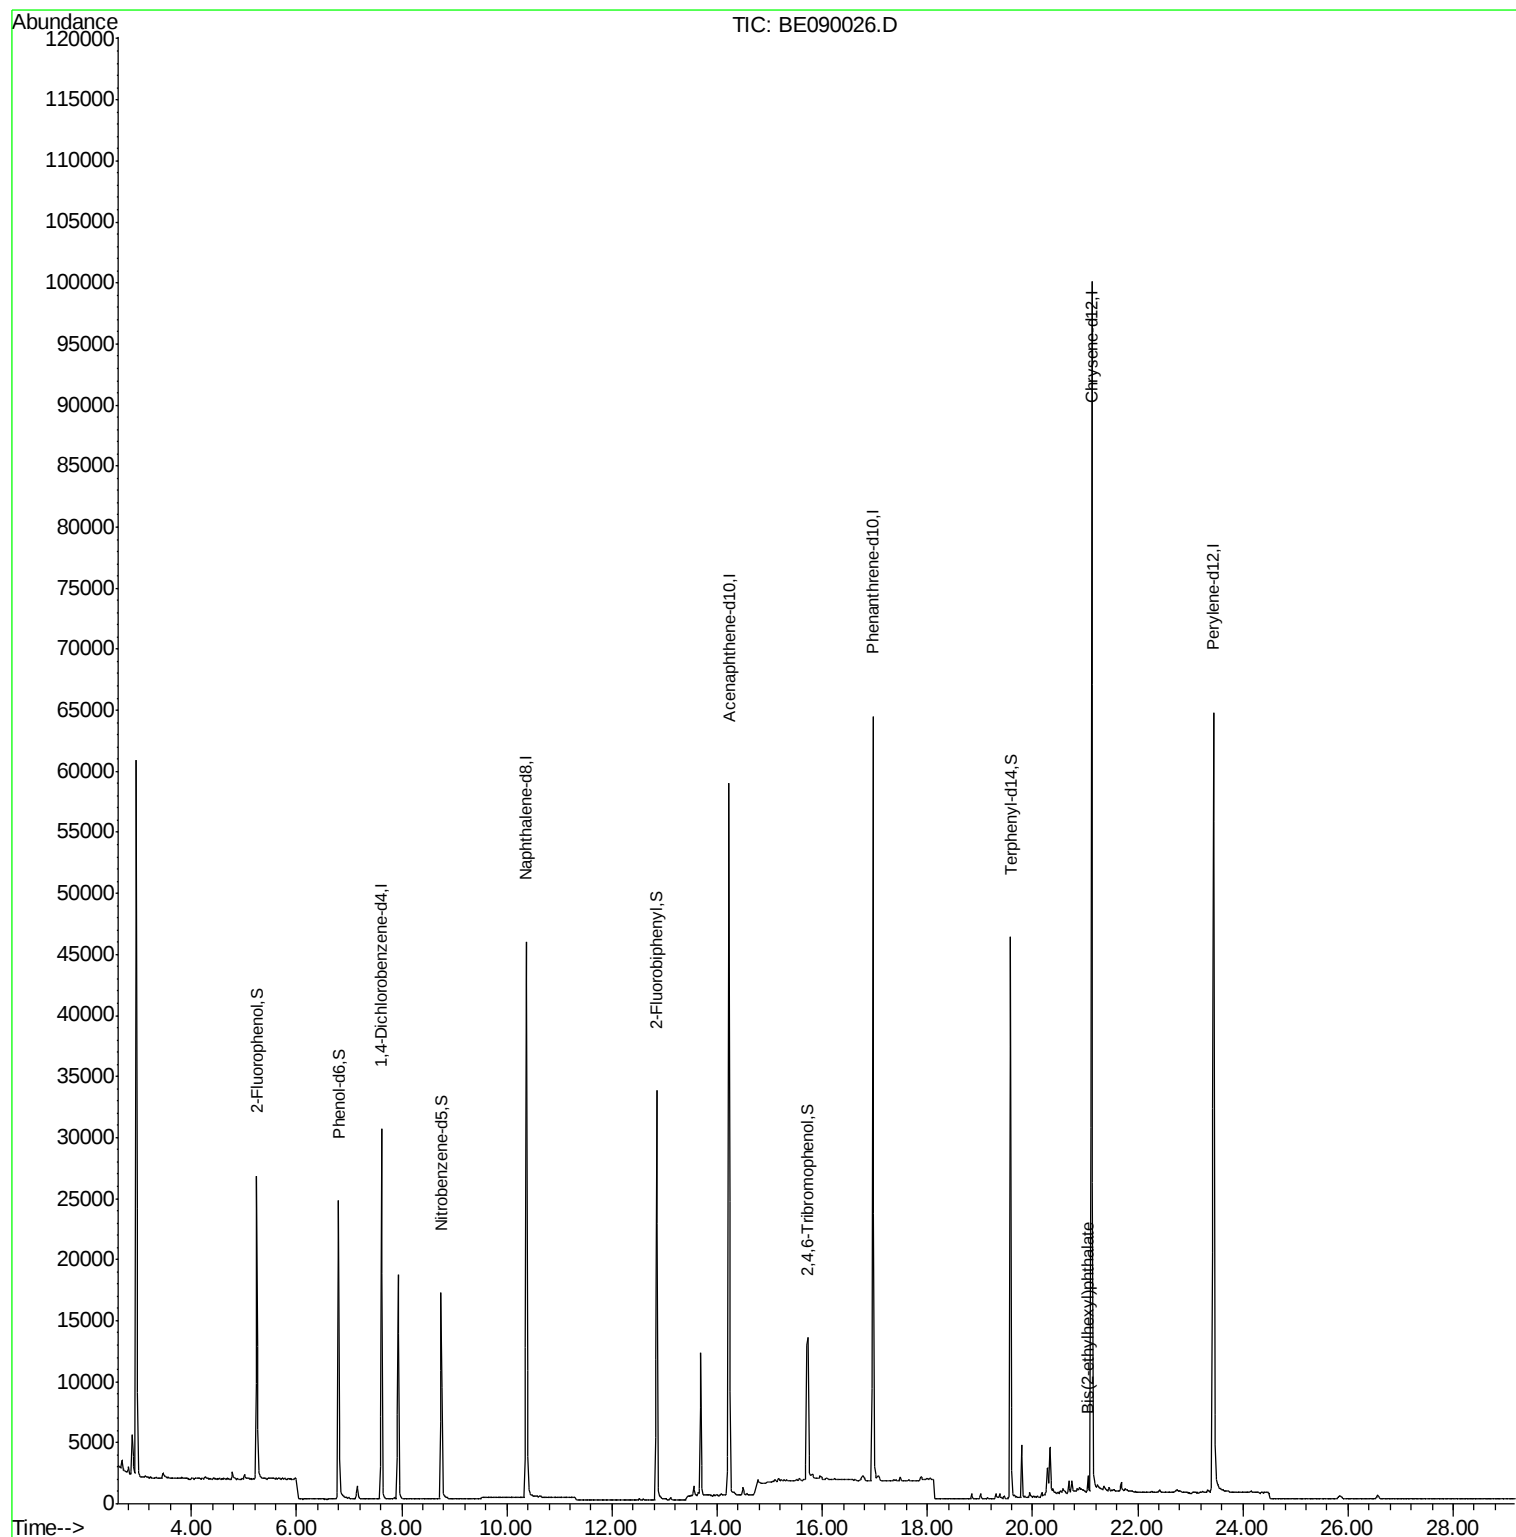




#1




1,4-Dichlorobenzene-d4  
Concen: 5.00 ng  
RT: 7.62 min Scan# 852  
Delta R.T. -0.01 min  
Lab File: BE090026.D  
Acq: 1 Jul 2015 00:32

Instrument :  
BNA\_E  
ClientSampleId :  
X1SB0520204-150625

Tgt Ion:152 Resp: 14266  
Ion Ratio Lower Upper  
152 100  
150 155.2 123.9 185.9  
115 63.8 50.6 76.0

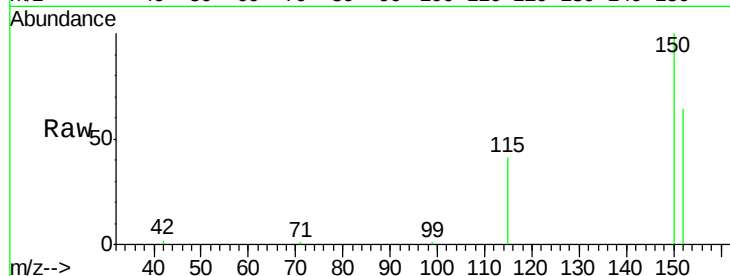


Abundance Ion 152.00 (151.70 to 152.70): E  
Ion 150.00 (149.70 to 150.70): E  
Ion 115.00 (114.70 to 115.70): E

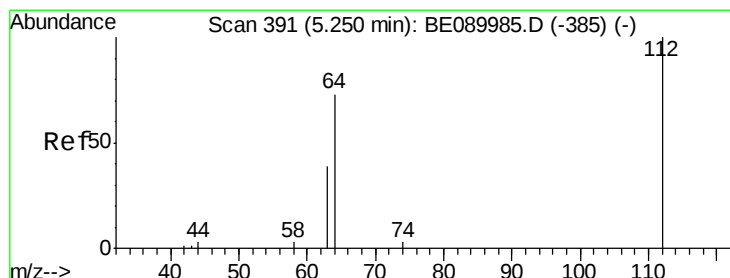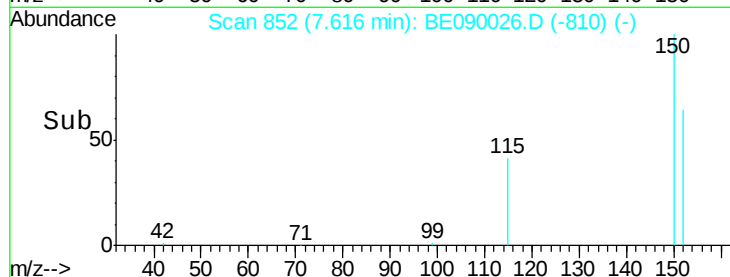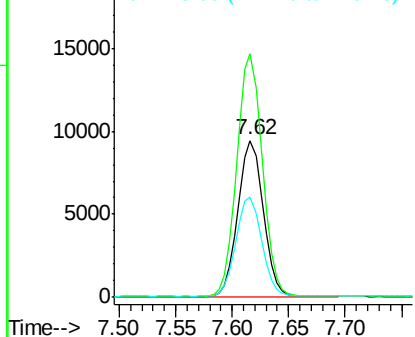



#4


2-Fluorophenol  
Concen: 5.47 ng  
RT: 5.24 min Scan# 390  
Delta R.T. -0.01 min  
Lab File: BE090026.D  
Acq: 1 Jul 2015 00:32

Tgt Ion:112 Resp: 17911  
Ion Ratio Lower Upper  
112 100  
64 69.7 56.3 84.5  
63 36.4 29.8 44.6

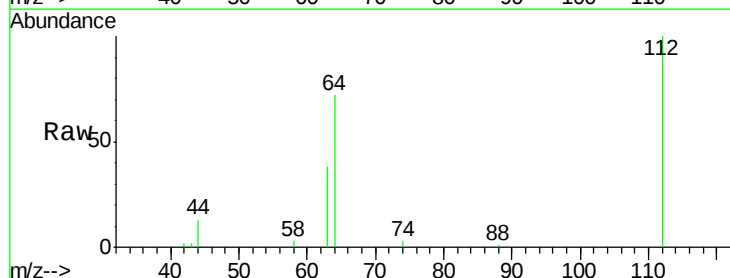

Abundance Ion 112.00 (111.70 to 112.70): E  
Ion 64.00 (63.70 to 64.70): BE0  
Ion 63.00 (62.70 to 63.70): BE0

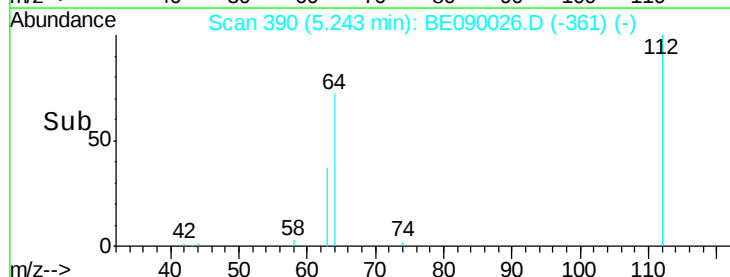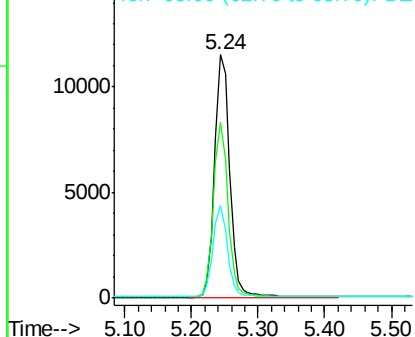

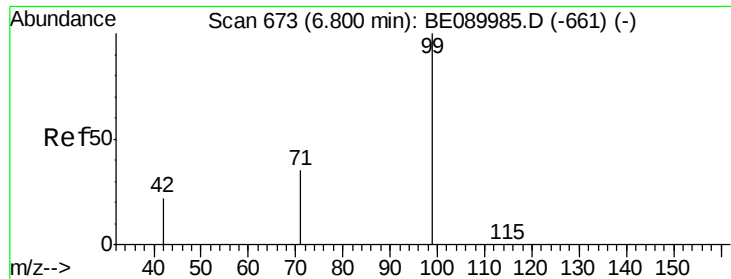

#5

Phenol-d6

Concen: 5.70 ng

RT: 6.80 min Scan# 672

Delta R.T. -0.00 min

Lab File: BE090026.D

Acq: 1 Jul 2015 00:32

Instrument :

BNA\_E

ClientSampleId :

X1SB0520204-150625





Tgt Ion: 99 Resp: 26141

Ion Ratio Lower Upper

99 100

42 20.0 18.7 28.1

71 33.6 27.5 41.3

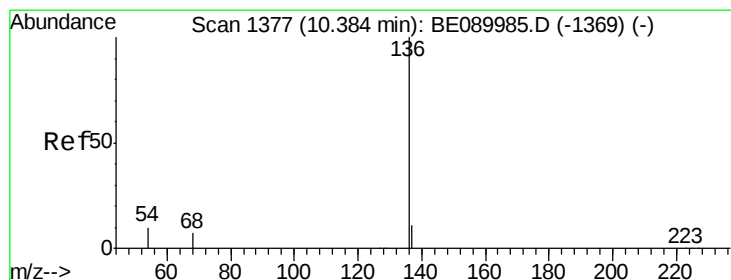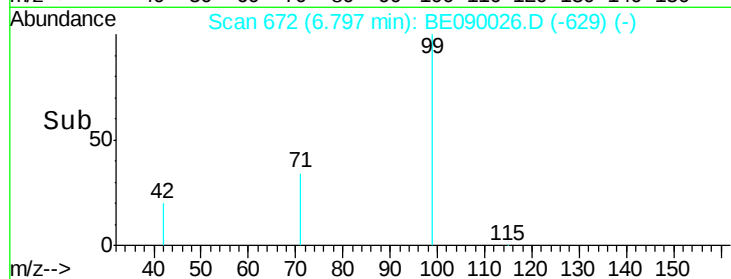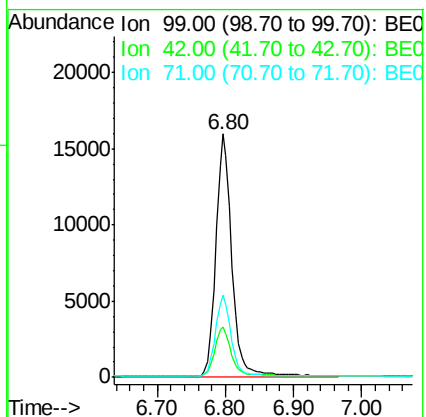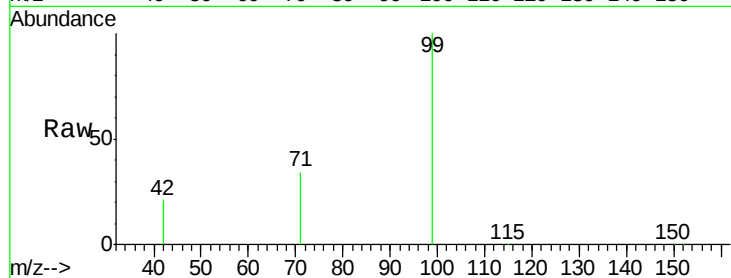

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.37 min Scan# 1375

Delta R.T. -0.01 min

Lab File: BE090026.D

Acq: 1 Jul 2015 00:32

Tgt Ion: 136 Resp: 61936




Ion Ratio Lower Upper


136 100

137 11.0 8.9 13.3

54 11.9 8.2 12.4

68 8.7 5.8 8.8

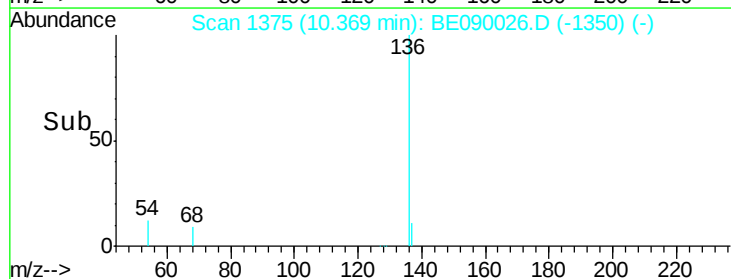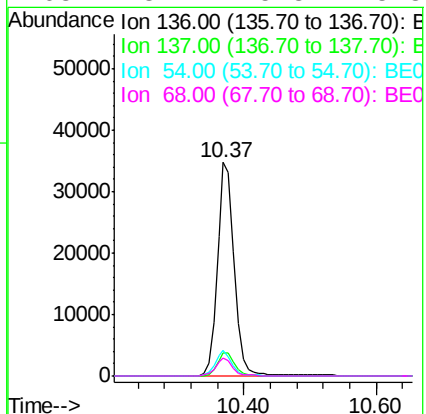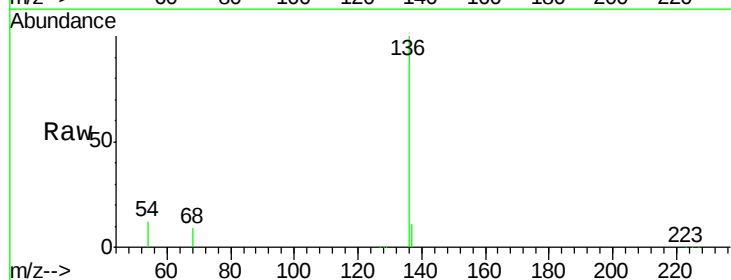

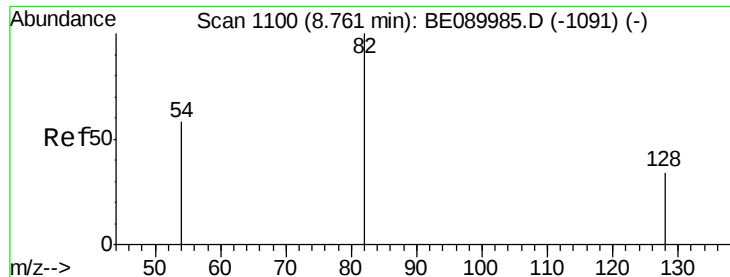

#7

Nitrobenzene-d5

Concen: 3.08 ng

RT: 8.75 min Scan# 1098

Delta R.T. -0.01 min

Lab File: BE090026.D

Acq: 1 Jul 2015 00:32

Instrument :

BNA\_E

ClientSampleId :

X1SB0520204-150625


Tgt Ion: 82 Resp: 15173

Ion Ratio Lower Upper




82 100

128 33.5 28.0 42.0

54 58.0 47.6 71.4

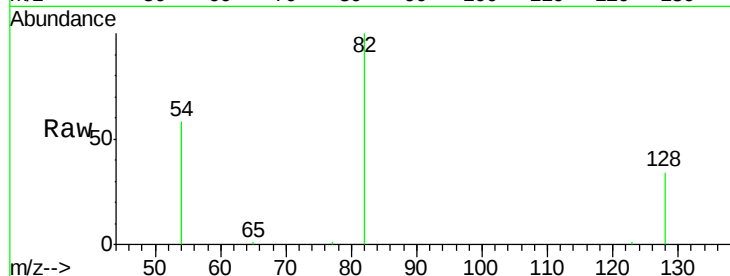

Abundance Ion 82.00 (81.70 to 82.70): BE0  
Ion 128.00 (127.70 to 128.70): BE0  
Ion 54.00 (53.70 to 54.70): BE0

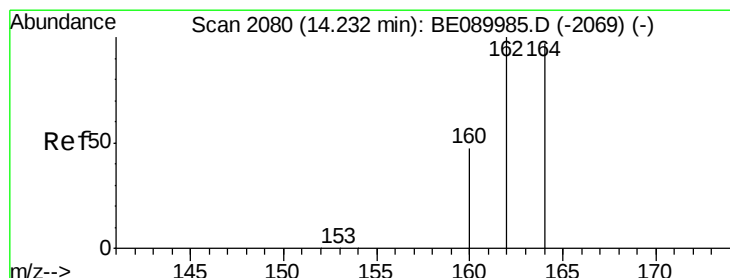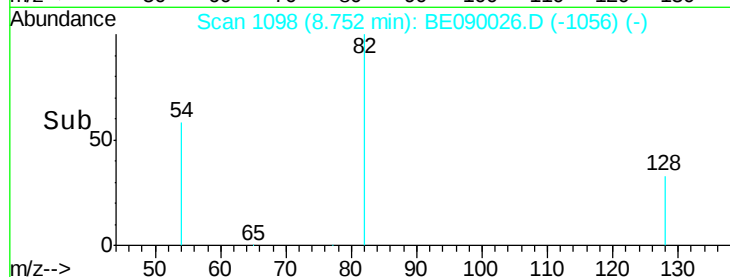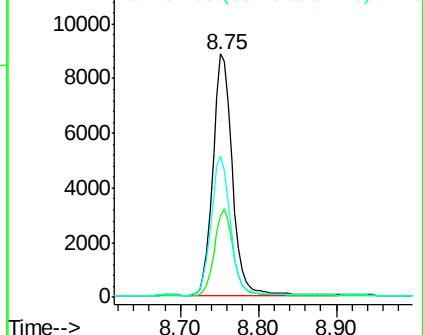

#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.22 min Scan# 2079

Delta R.T. -0.01 min

Lab File: BE090026.D

Acq: 1 Jul 2015 00:32


Tgt Ion: 164 Resp: 34435

Ion Ratio Lower Upper



164 100


162 104.2 82.2 123.4

160 47.9 39.0 58.6

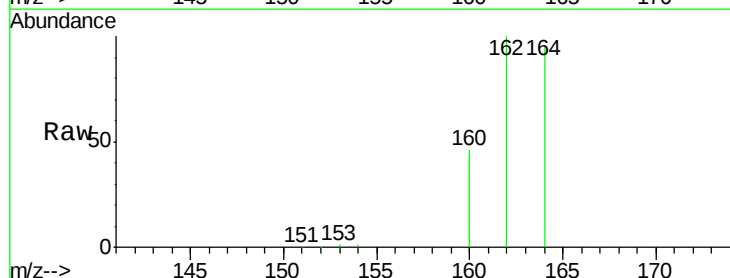

Abundance Ion 164.00 (163.70 to 164.70): E  
Ion 162.00 (161.70 to 162.70): E  
Ion 160.00 (159.70 to 160.70): E



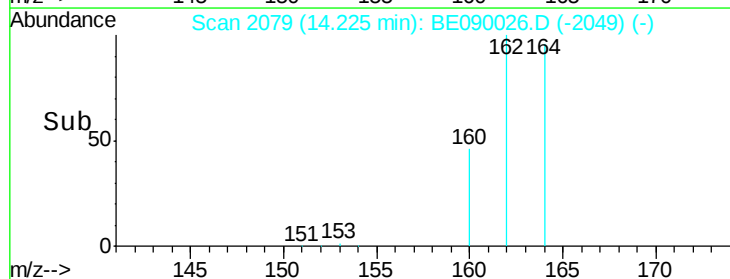
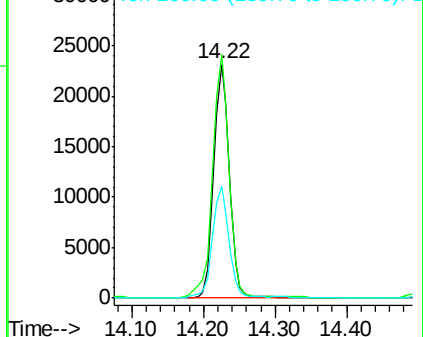


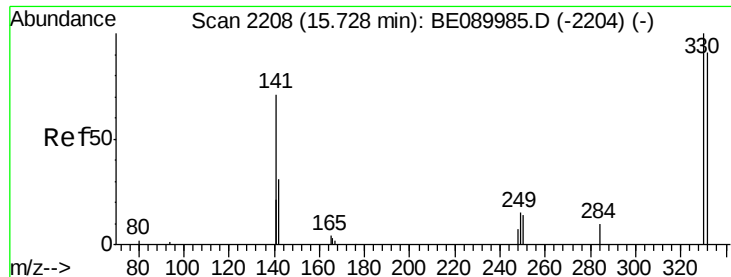

#13  
 2,4,6-Tribromophenol  
 Concen: 6.26 ng  
 RT: 15.73 min Scan# 2208  
 Delta R.T. -0.00 min  
 Lab File: BE090026.D  
 Acq: 1 Jul 2015 00:32




Instrument :  
 BNA\_E  
 ClientSampleId :  
 X1SB0520204-150625


Tgt Ion: 330 Resp: 6321  
 Ion Ratio Lower Upper  
 330 100  
 332 97.4 76.4 114.6  
 141 171.6 130.3 195.5

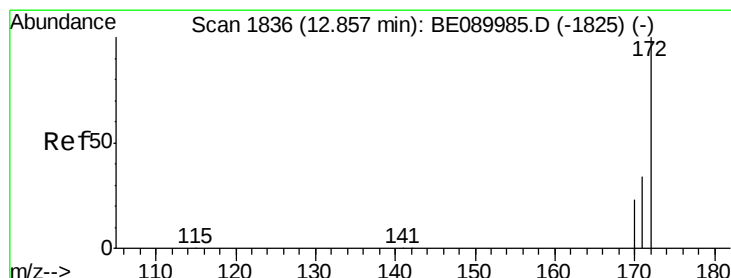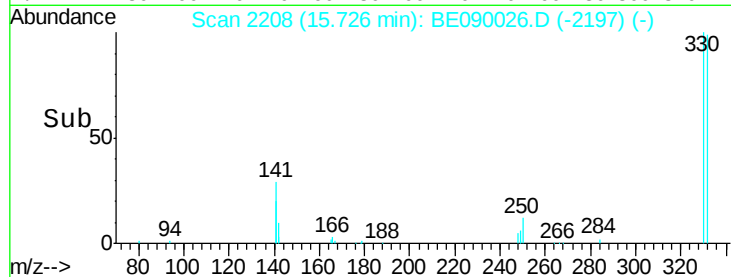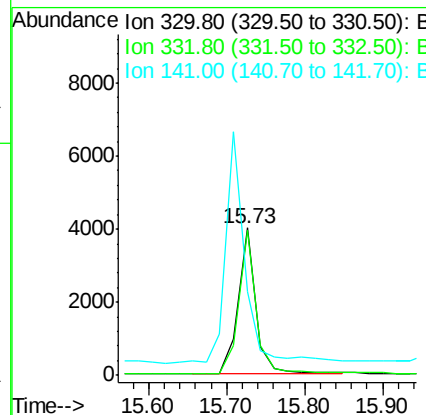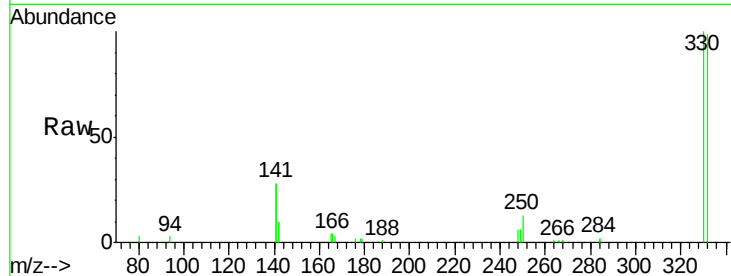

#14  
 2-Fluorobiphenyl  
 Concen: 3.12 ng  
 RT: 12.85 min Scan# 1834  
 Delta R.T. -0.01 min  
 Lab File: BE090026.D  
 Acq: 1 Jul 2015 00:32

Tgt Ion: 172 Resp: 32318  
 Ion Ratio Lower Upper  
 172 100  
 171 34.2 27.8 41.6  
 170 23.4 18.3 27.5

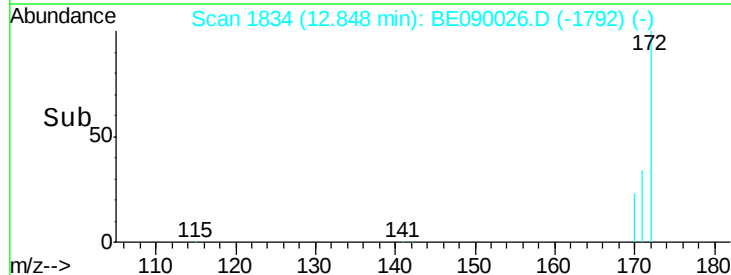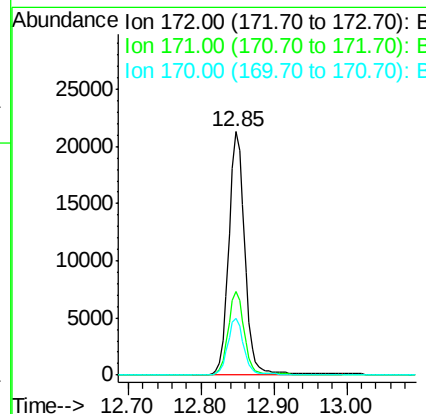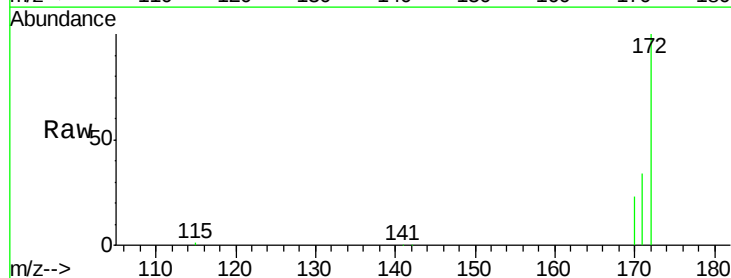

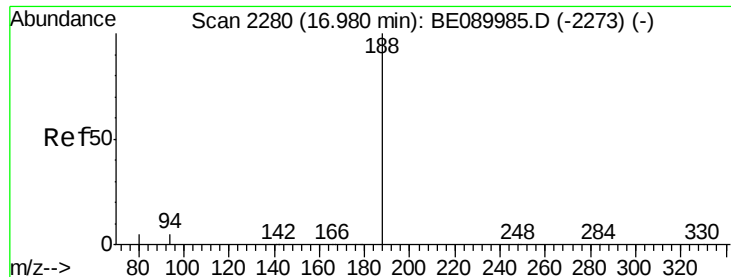

#18

Phenanthrene-d10

Concen: 5.00 ng

RT: 16.96 min Scan# 2279

Delta R.T. -0.02 min

Lab File: BE090026.D

Acq: 1 Jul 2015 00:32

Instrument :

BNA\_E

ClientSampleId :

X1SB0520204-150625


Tgt Ion:188 Resp: 77640

Ion Ratio Lower Upper

188 100

94 13.3 4.1 6.1#




80 14.6 4.2 6.2#

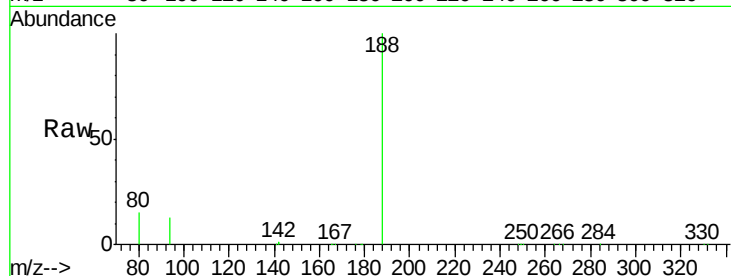

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

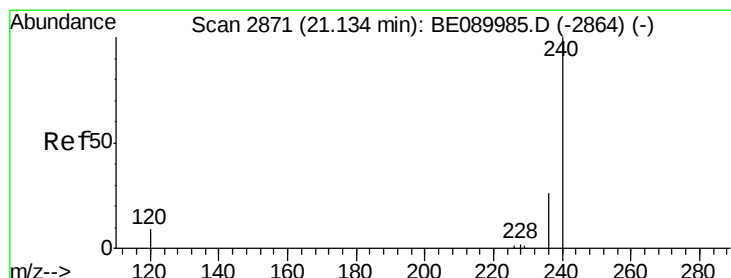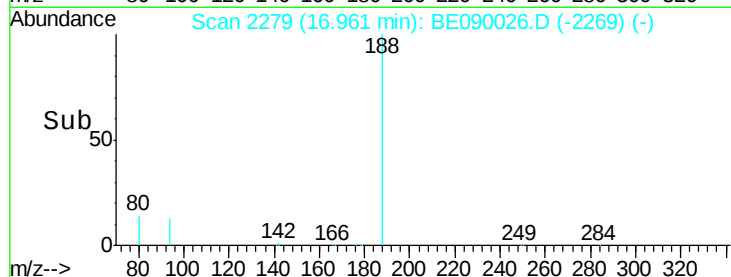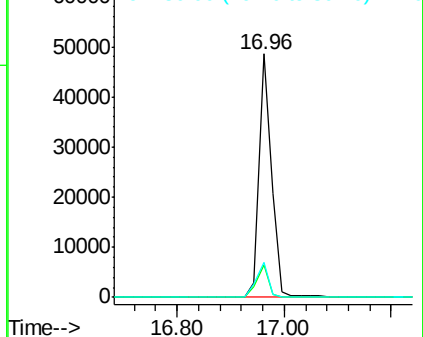

#25

Chrysene-d12

Concen: 5.00 ng

RT: 21.12 min Scan# 2869

Delta R.T. -0.01 min

Lab File: BE090026.D

Acq: 1 Jul 2015 00:32


Tgt Ion:240 Resp: 93223

Ion Ratio Lower Upper

240 100

120 10.8 6.9 10.3#



236 26.5 20.8 31.2

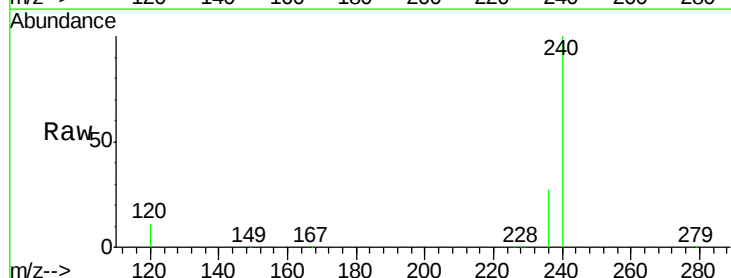


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



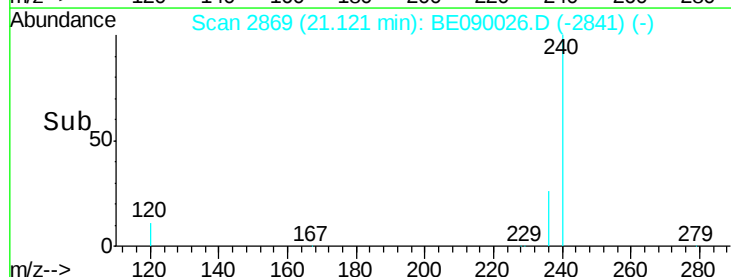
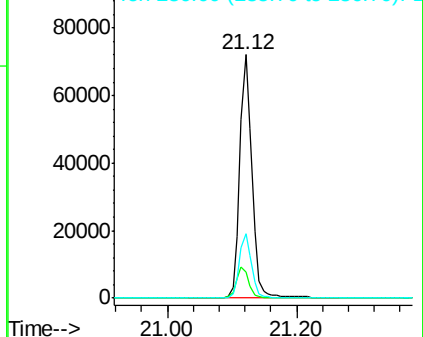


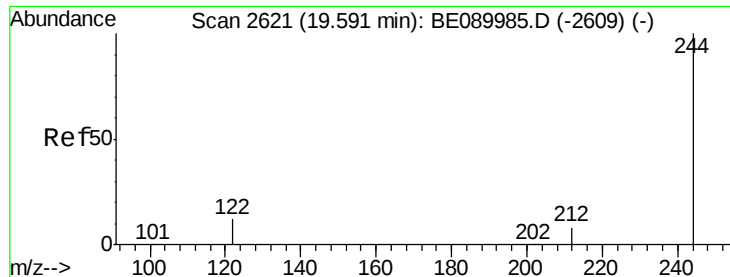

#27  
 Terphenyl-d14  
 Concen: 3.02 ng  
 RT: 19.58 min Scan# 2619  
 Delta R.T. -0.01 min  
 Lab File: BE090026.D  
 Acq: 1 Jul 2015 00:32




Instrument :  
 BNA\_E  
 ClientSampleId :  
 X1SB0520204-150625



Tgt Ion: 244 Resp: 46851  
 Ion Ratio Lower Upper  
 244 100  
 212 8.0 6.6 9.8  
 122 13.0 9.8 14.8

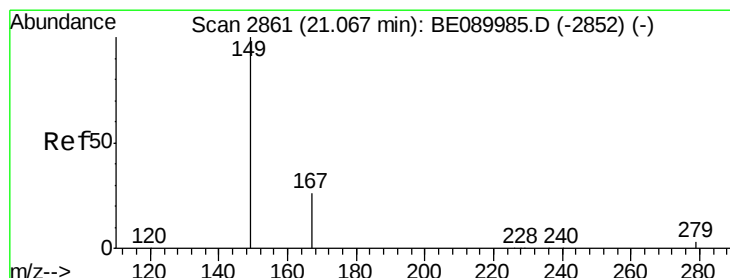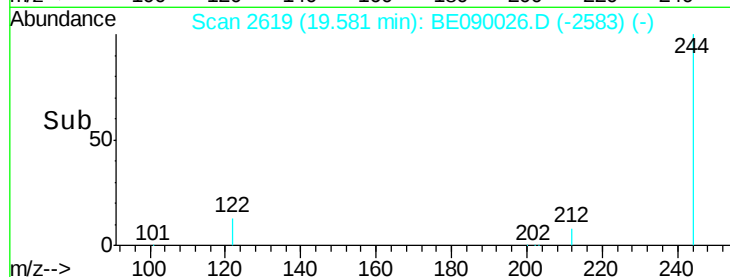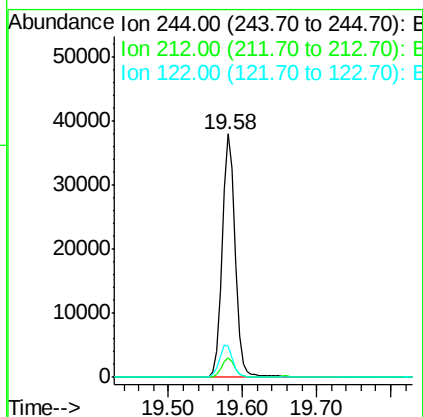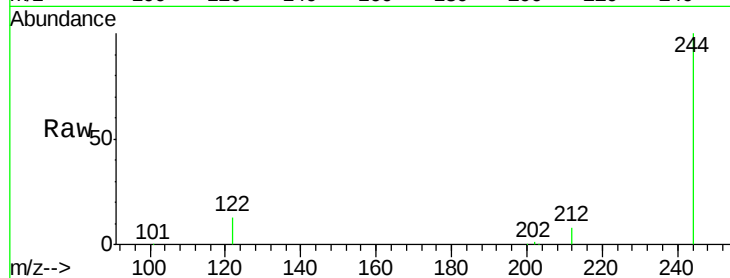

#30  
 Bis(2-ethylhexyl)phthalate  
 Concen: 0.40 ng  
 RT: 21.05 min Scan# 2859  
 Delta R.T. -0.01 min  
 Lab File: BE090026.D  
 Acq: 1 Jul 2015 00:32

Tgt Ion: 149 Resp: 1031  
 Ion Ratio Lower Upper  
 149 100  
 167 28.9 20.3 30.5  
 279 4.3 2.6 3.8#

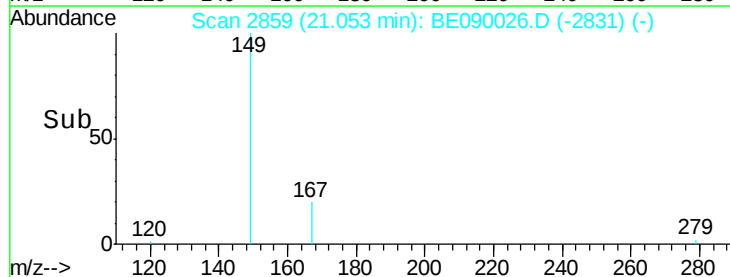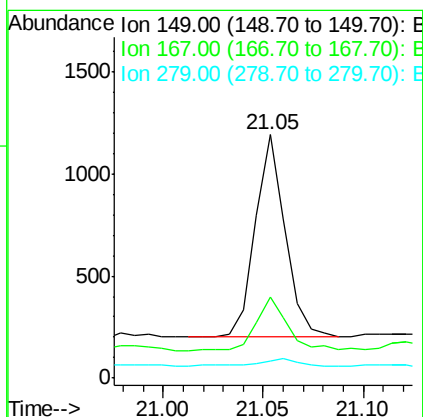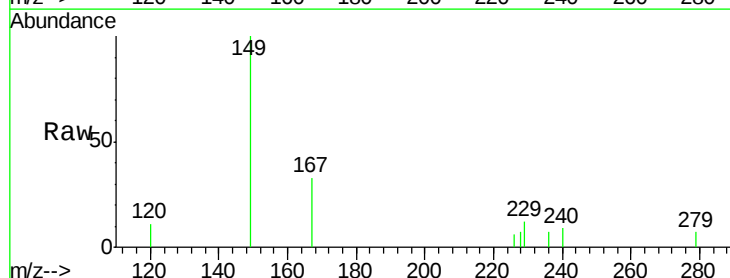

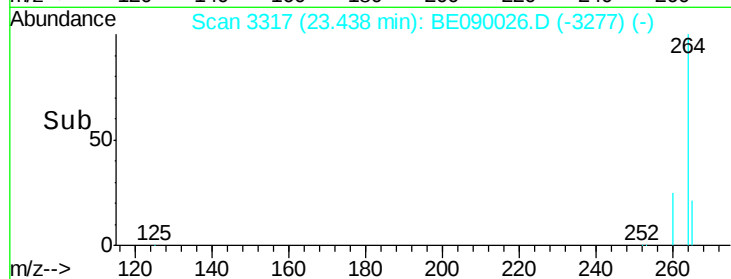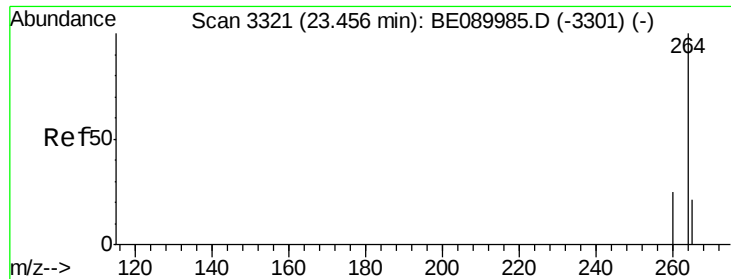

#32

Perylene-d12

Concen: 5.00 ng

RT: 23.44 min Scan# 3317

Delta R.T. -0.02 min

Lab File: BE090026.D

Acq: 1 Jul 2015 00:32

Instrument :

BNA\_E

ClientSampleId :

X1SB0520204-150625

Tgt Ion:264 Resp: 90293

Ion Ratio Lower Upper

264 100

260 25.0 20.2 30.2

265 22.0 17.1 25.7

