


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE063015\
 Data File : BE090012.D
 Acq On : 30 Jun 2015 15:35
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BE062915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 30 07:01:01 2015

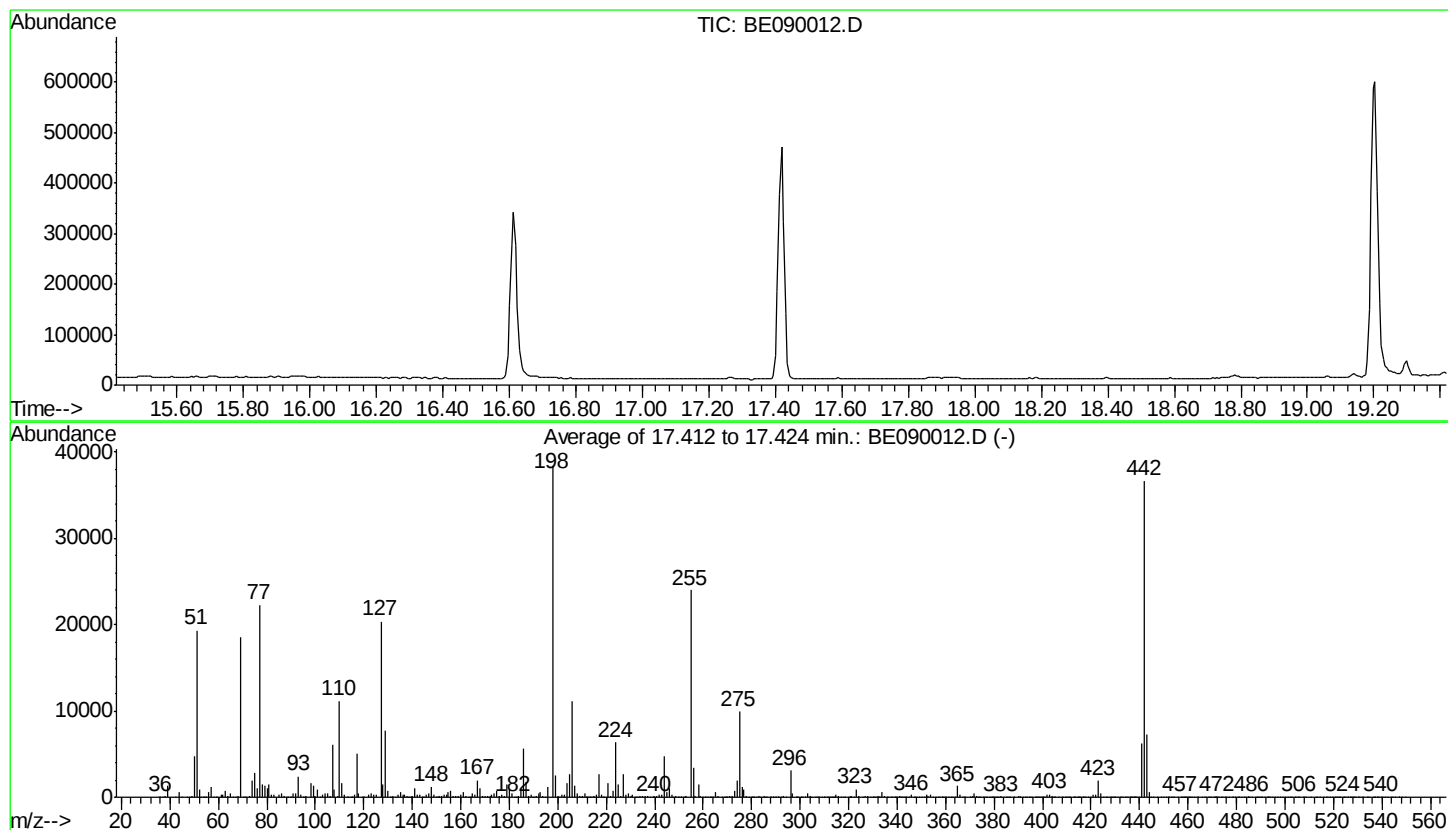

AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.3	19292	PASS
68	69	0.00	2	1.1	206	PASS
69	198	0.00	100	48.2	18515	PASS
70	69	0.00	2	0.3	59	PASS
127	198	10	80	53.0	20341	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38376	PASS
199	198	5	9	6.6	2551	PASS
275	198	10	60	25.8	9920	PASS
365	198	1	100	3.4	1309	PASS
441	442	0.01	24	16.9	6183	PASS
442	198	50	100	95.4	36618	PASS
443	442	15	24	19.6	7192	PASS