


Data Path : Z:\HPCHEM1\BNA_E\Data\BE063015\
 Data File : BE090028.D
 Acq On : 1 Jul 2015 2:20
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BE062915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 30 07:01:01 2015

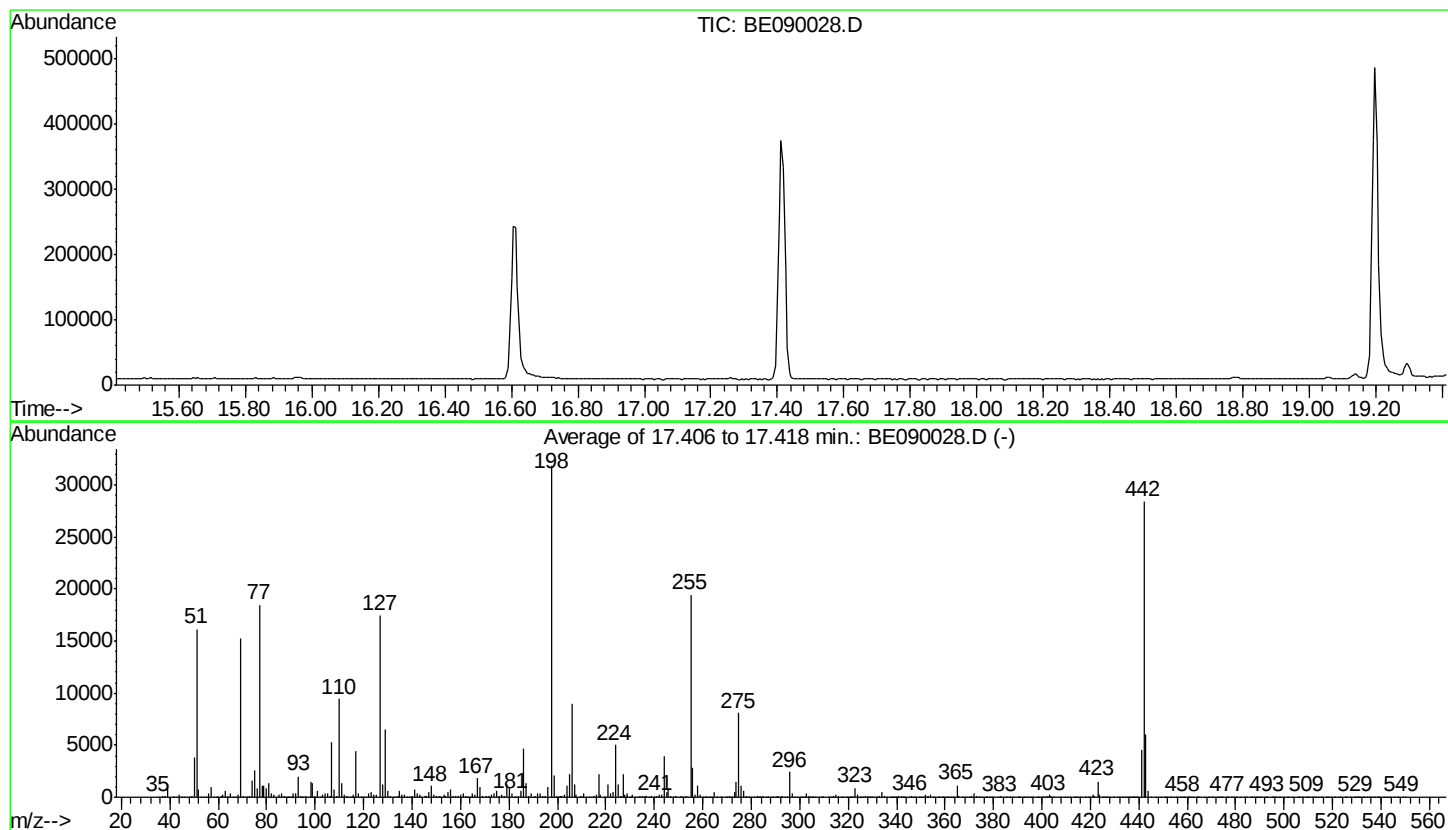

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.7	16169	PASS
68	69	0.00	2	1.4	212	PASS
69	198	0.00	100	47.8	15244	PASS
70	69	0.00	2	0.5	71	PASS
127	198	10	80	54.8	17446	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31861	PASS
199	198	5	9	6.5	2062	PASS
275	198	10	60	25.5	8115	PASS
365	198	1	100	3.6	1161	PASS
441	442	0.01	24	16.0	4546	PASS
442	198	50	100	89.2	28408	PASS
443	442	15	24	21.4	6069	PASS