


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE070115\
Data File : BE090041.D
Acq On : 1 Jul 2015 10:48
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BE062915.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 30 07:01:01 2015

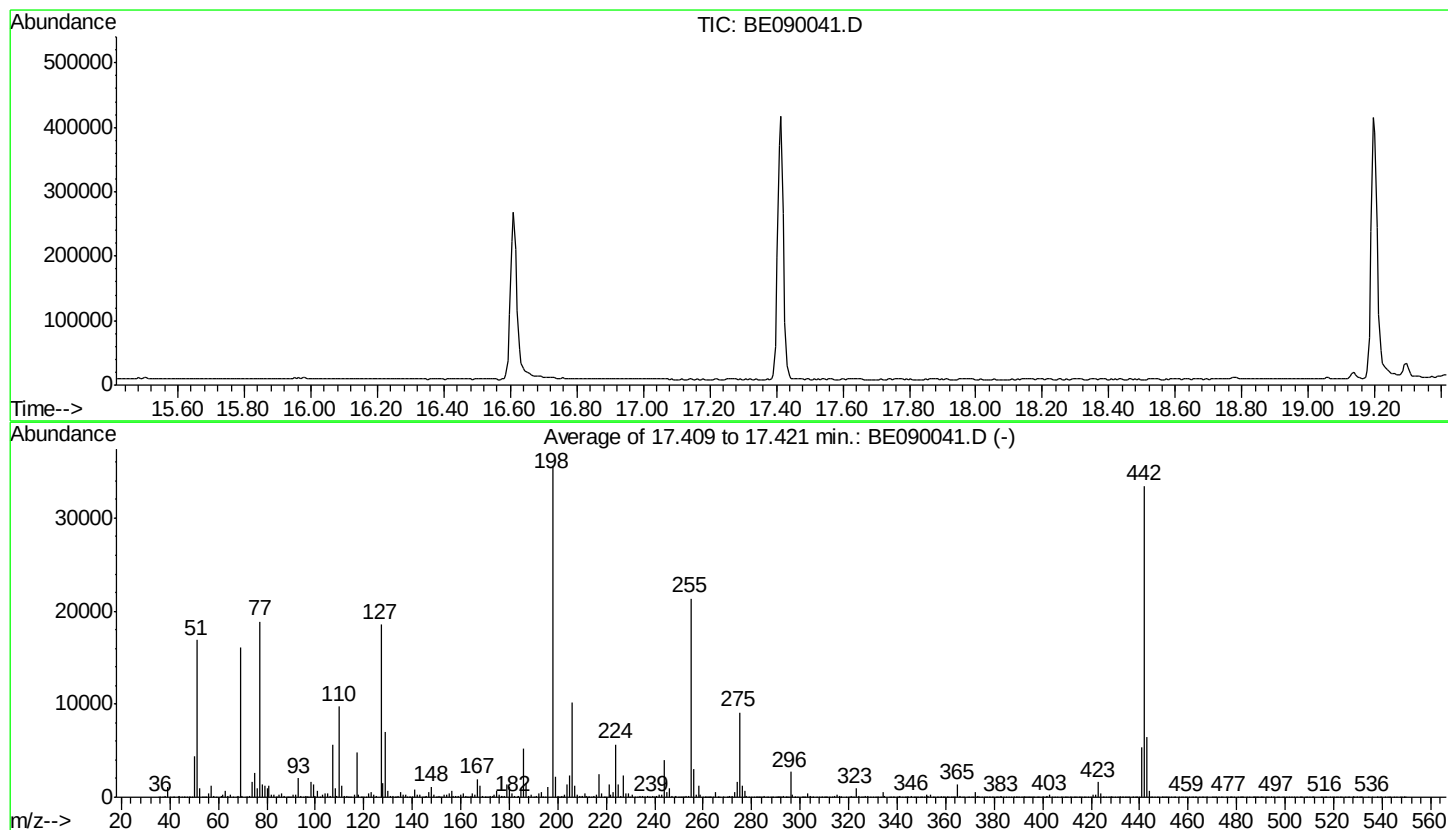

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.4	16877	PASS
68	69	0.00	2	1.0	156	PASS
69	198	0.00	100	45.2	16120	PASS
70	69	0.00	2	0.6	89	PASS
127	198	10	80	52.0	18543	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	35634	PASS
199	198	5	9	6.4	2266	PASS
275	198	10	60	25.6	9129	PASS
365	198	1	100	3.8	1349	PASS
441	442	0.01	24	16.2	5436	PASS
442	198	50	100	94.0	33492	PASS
443	442	15	24	19.5	6538	PASS