


Data Path : Z:\HPCHEM1\BNA_E\Data\BE070117\
 Data File : BE093376.D
 Acq On : 30 Jun 2017 14:00
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE070117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jul 01 15:43:24 2017

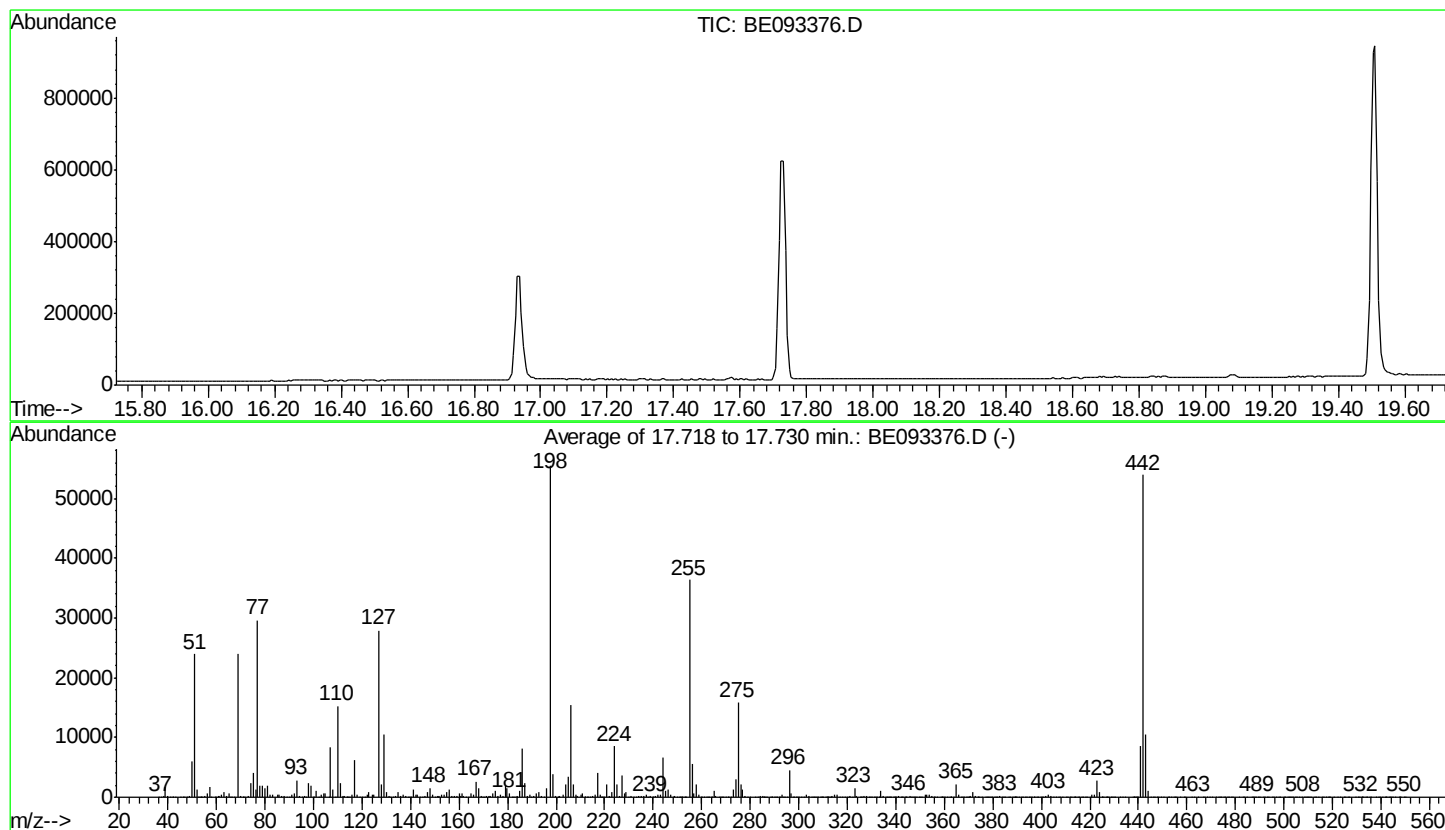

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2568

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	23958	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.4	24065	PASS
70	69	0.00	2	0.7	176	PASS
127	198	10	80	50.4	27941	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55480	PASS
199	198	5	9	7.0	3858	PASS
275	198	10	60	28.5	15807	PASS
365	198	1	100	4.0	2233	PASS
441	442	0.01	24	15.8	8517	PASS
442	198	50	100	97.1	53891	PASS
443	442	15	24	19.6	10548	PASS