


Data Path : Z:\HPCHEM1\BNA_E\Data\BE070117\
Data File : BE093385.D
Acq On : 1 Jul 2017 10:30
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE070117.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jul 01 15:43:24 2017

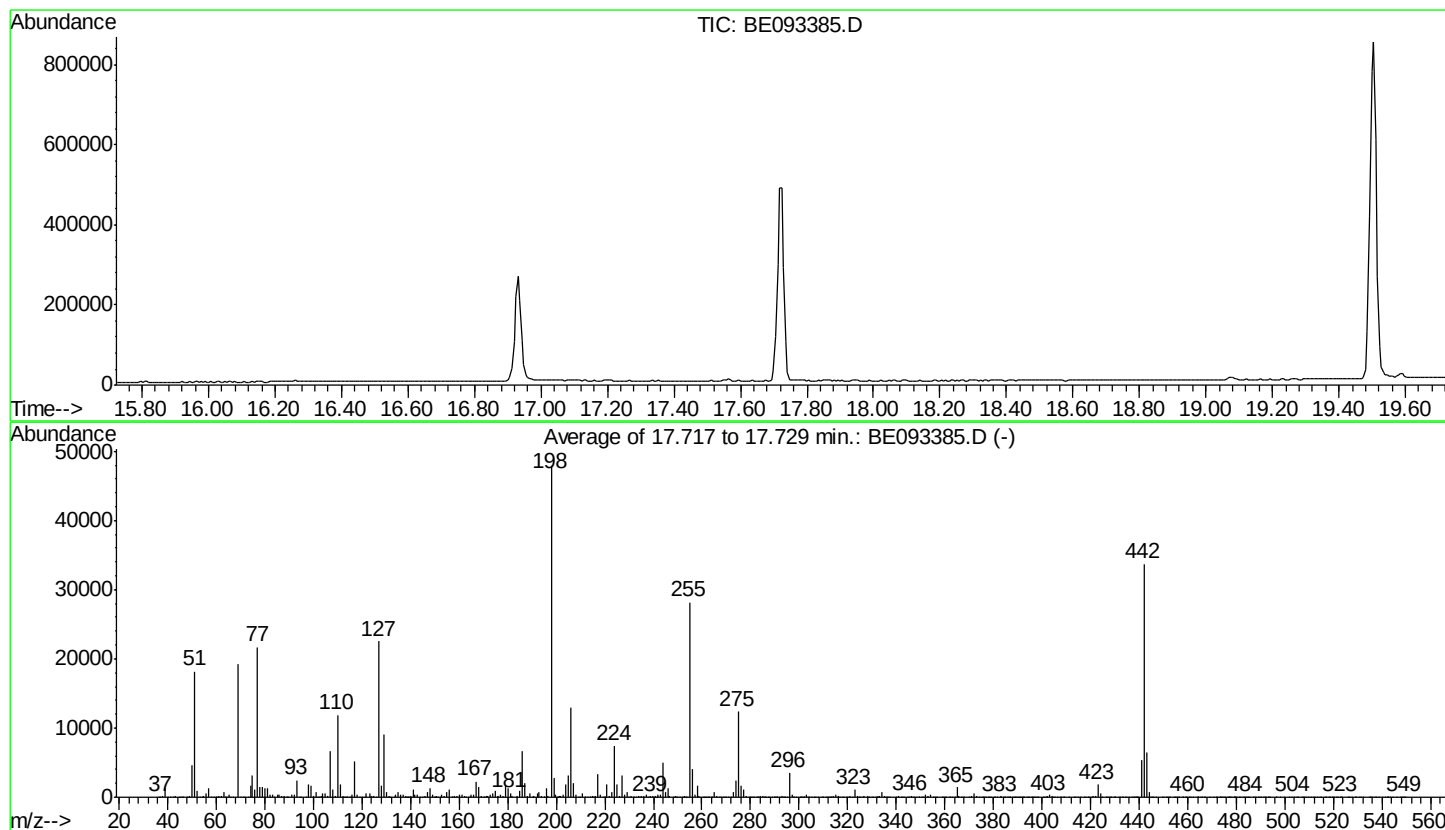

AutoFind: Scans 2575, 2576, 2577; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	18176	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.0	19174	PASS
70	69	0.00	2	0.4	80	PASS
127	198	10	80	47.0	22536	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	47920	PASS
199	198	5	9	6.0	2855	PASS
275	198	10	60	25.7	12326	PASS
365	198	1	100	3.1	1474	PASS
441	442	0.01	24	16.2	5451	PASS
442	198	50	100	70.3	33689	PASS
443	442	15	24	19.0	6397	PASS