


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE070215\
Data File : BE090050.D
Acq On : 2 Jul 2015 9:38
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BE062915.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 30 07:01:01 2015

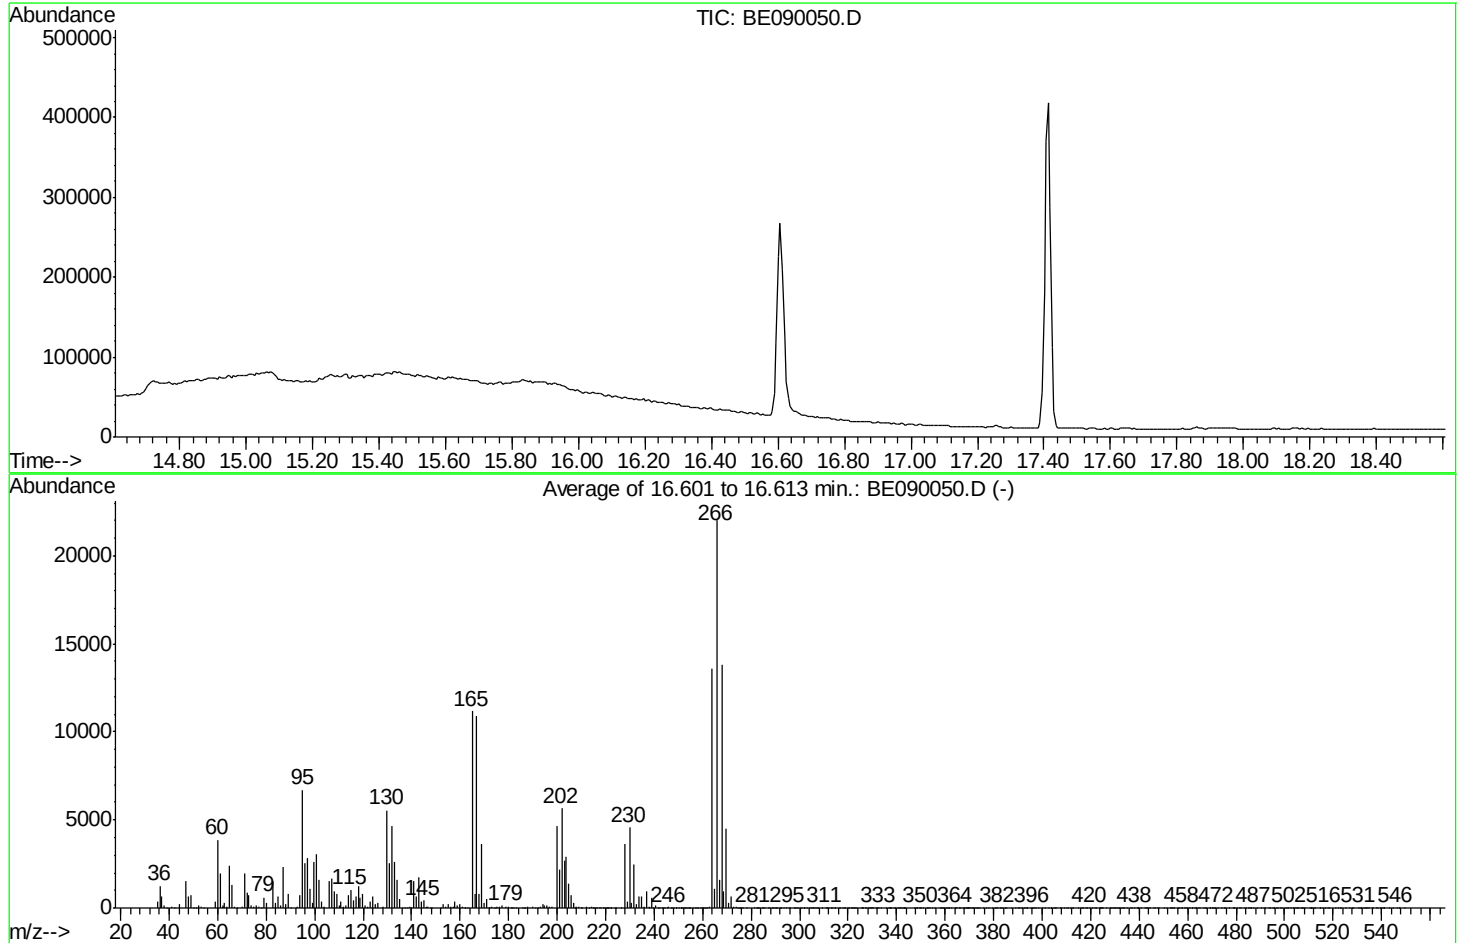

AutoFind: Scans 2385, 2386, 2387; Background Corrected with Scan 2379

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	0.2	11	FAIL *
75	95	30	60	0.6	39	FAIL *
95	95	100	100	100.0	6719	PASS
96	95	5	9	37.5	2520	FAIL *
173	174	0.00	2	215.8	41	FAIL *
174	95	50	100	0.3	19	FAIL *
175	174	5	9	294.7	56	FAIL *
176	174	95	101	252.6	48	FAIL *
177	176	5	9	262.5	126	FAIL *