


Data Path : Z:\HPCHEM1\BNA_E\Data\BE070217\
 Data File : BE093404.D
 Acq On : 2 Jul 2017 9:03
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE070217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 03 06:40:23 2017

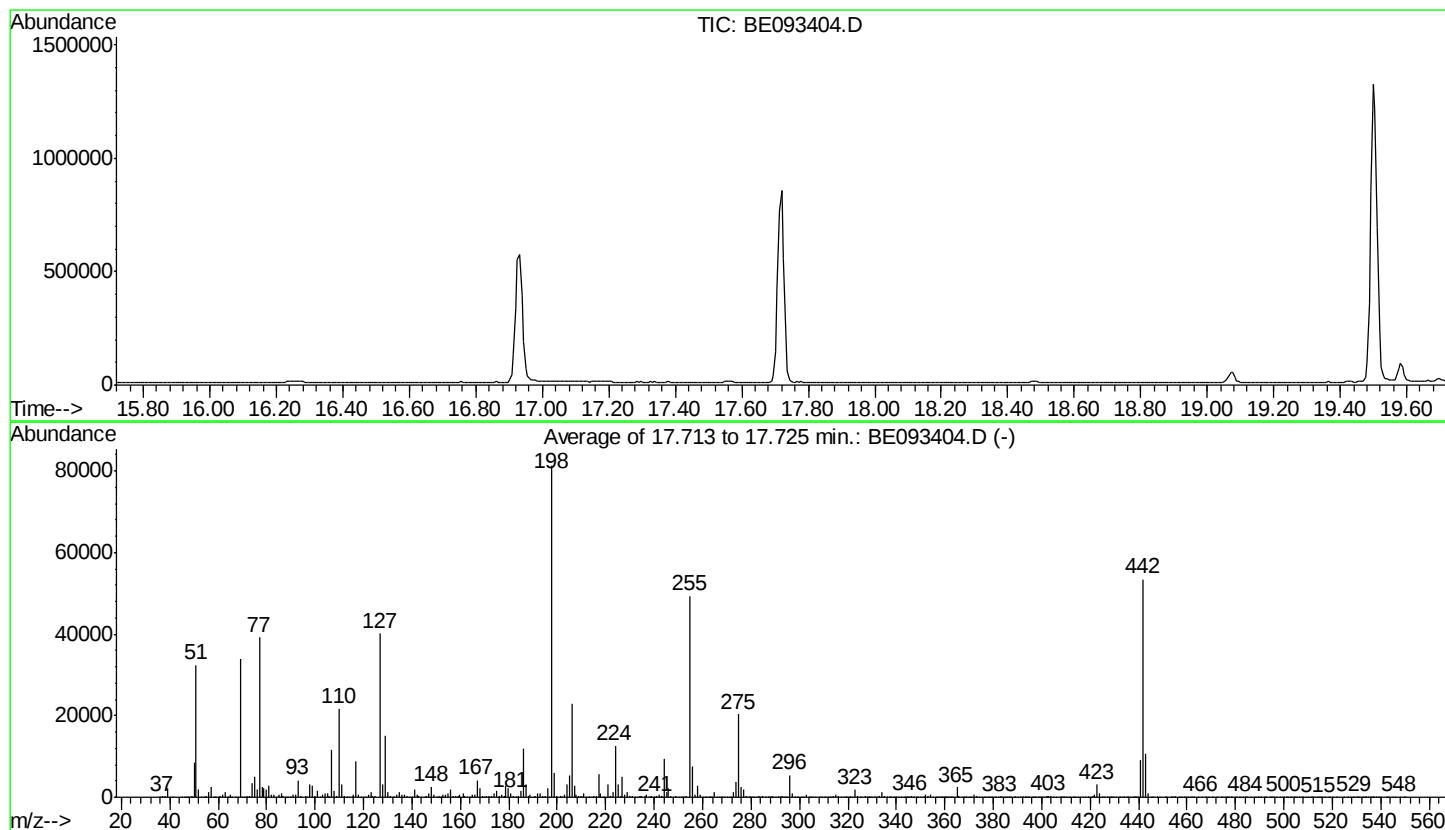

AutoFind: Scans 2574, 2575, 2576; Background Corrected with Scan 2565

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	32363	PASS
68	69	0.00	2	0.3	108	PASS
69	198	0.00	100	41.6	33815	PASS
70	69	0.00	2	0.4	147	PASS
127	198	10	80	49.3	40061	PASS
197	198	0.00	2	0.1	116	PASS
198	198	100	100	100.0	81316	PASS
199	198	5	9	7.3	5904	PASS
275	198	10	60	25.1	20386	PASS
365	198	1	100	3.1	2481	PASS
441	442	0.01	24	17.1	9130	PASS
442	198	50	100	65.8	53469	PASS
443	442	15	24	19.9	10644	PASS