
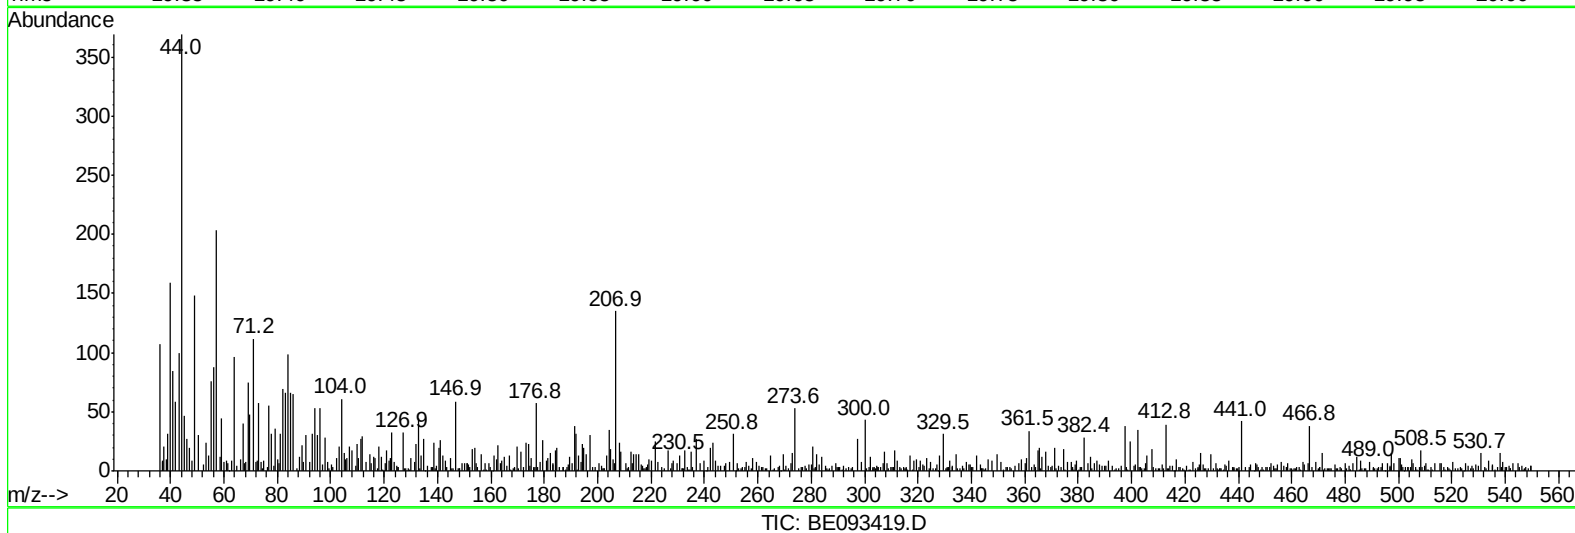


Data Path : Z:\HPCHEM1\BNA E\Data\BE070317\
Data File : BE093419.D
Acq On : 3 Jul 2017 8:42
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 04 05:13:53 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 03 01:43:12 2017
Response via : Initial Calibration

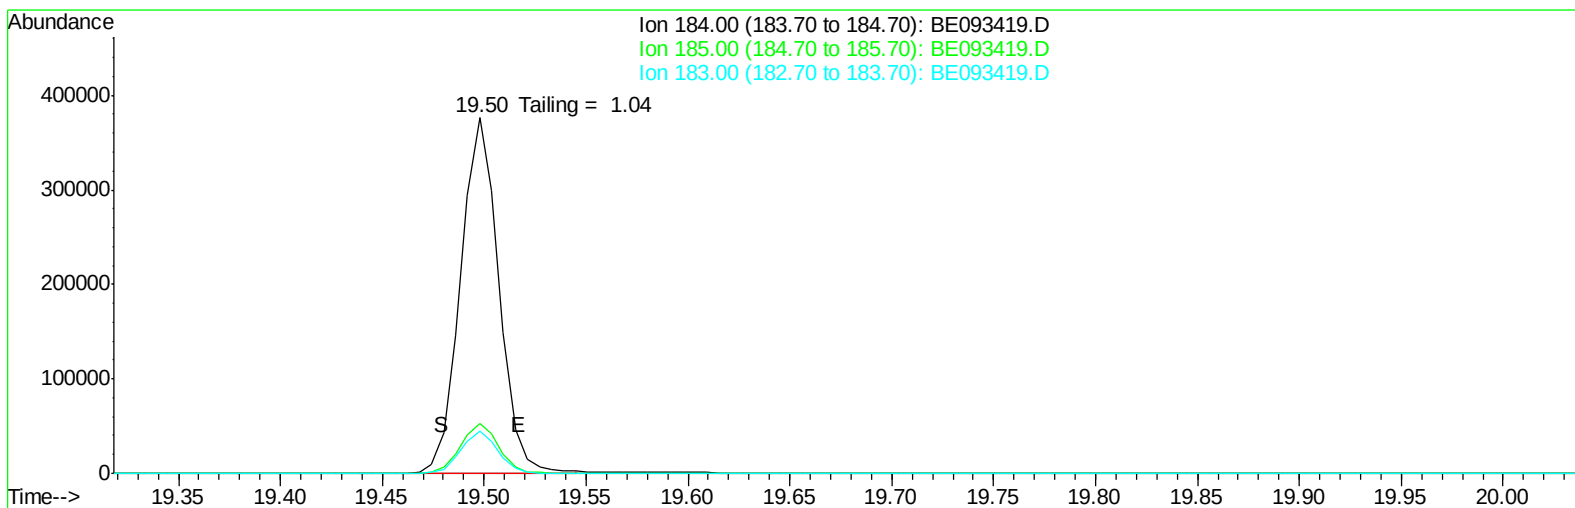

TIC: BE093419.D

(76) Benzidine



12.506min (-0.069) 26.97ng

response 22

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	8.33#
183.00	12.20	30.56#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA E\Data\BE070317\
Data File : BE093419.D
Acq On : 3 Jul 2017 8:42
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 04 05:13:53 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 03 01:43:12 2017
Response via : Initial Calibration

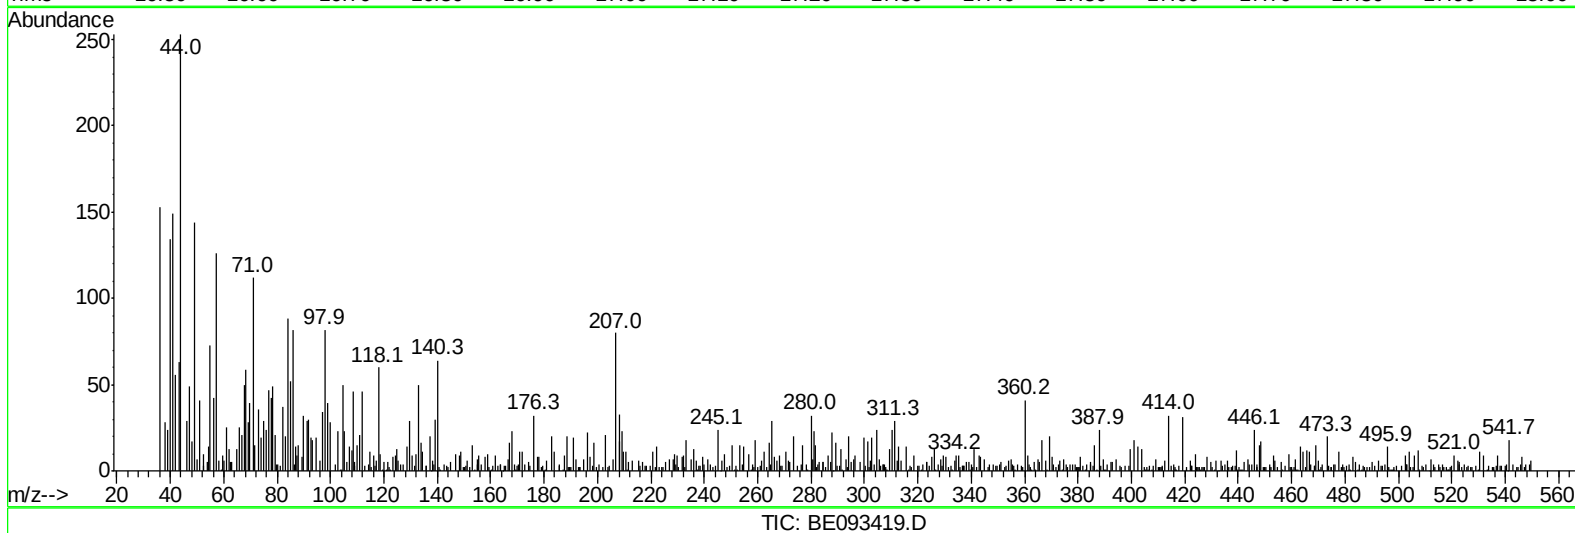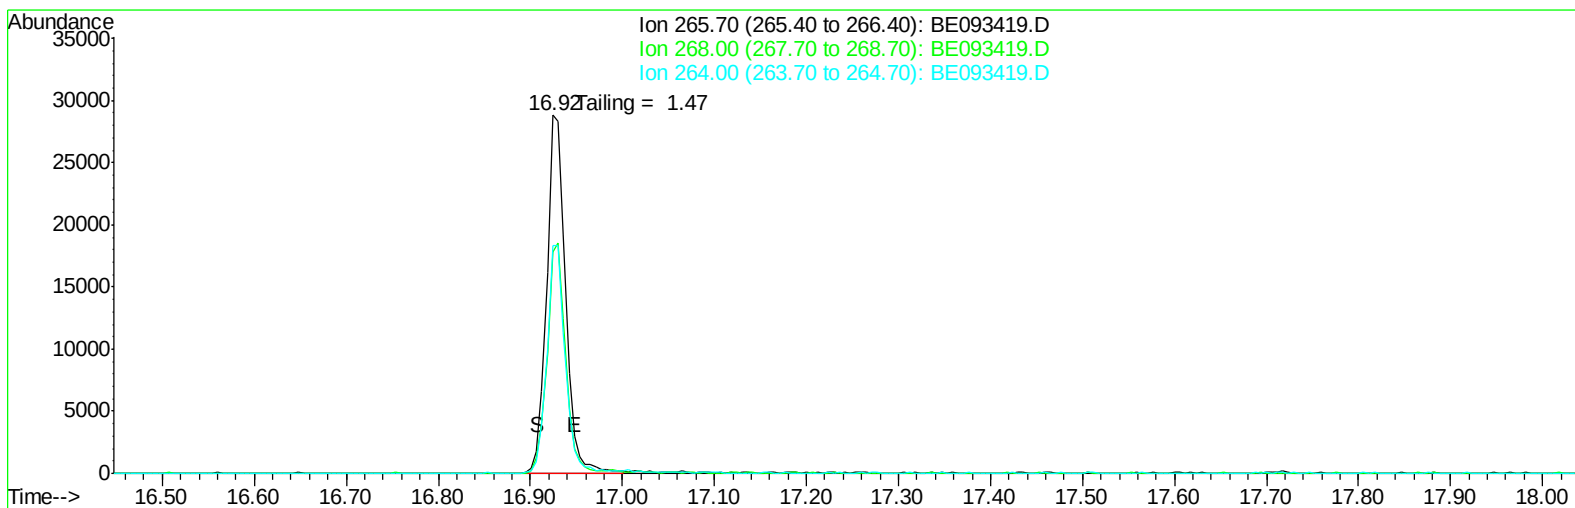

(69) Pentachlorophenol (C)

11.025min (-0.032) 769.06ng

response 34

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	24.32#
264.00	64.60	43.24#
0.00	0.00	0.00