


Data Path : Z:\HPCHEM1\BNA_E\Data\BE070317\
Data File : BE093419.D
Acq On : 3 Jul 2017 8:42
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE070217.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jul 03 06:40:23 2017

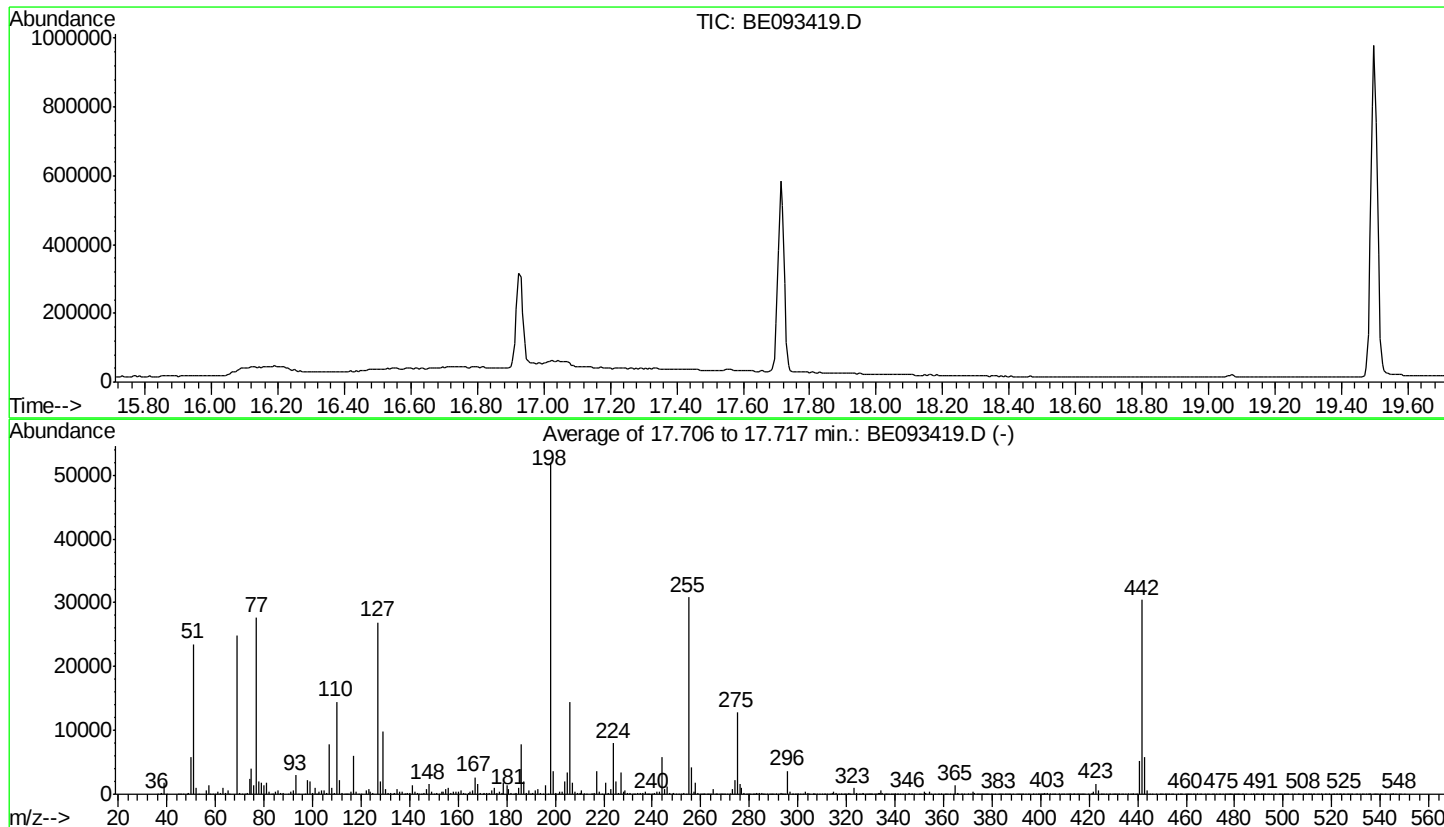

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2565

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.3	23518	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	47.9	24867	PASS
70	69	0.00	2	0.5	124	PASS
127	198	10	80	51.9	26937	PASS
197	198	0.00	2	0.1	63	PASS
198	198	100	100	100.0	51940	PASS
199	198	5	9	6.9	3564	PASS
275	198	10	60	24.6	12757	PASS
365	198	1	100	2.6	1374	PASS
441	442	0.01	24	17.0	5174	PASS
442	198	50	100	58.6	30415	PASS
443	442	15	24	19.0	5764	PASS