
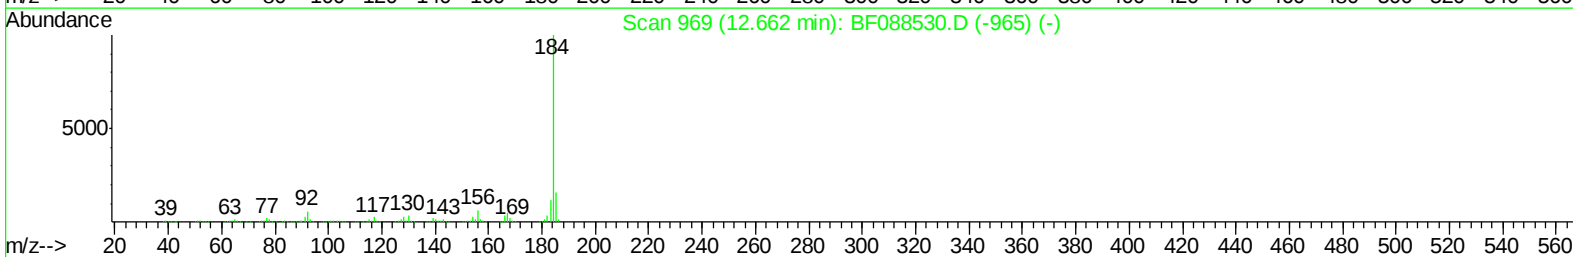
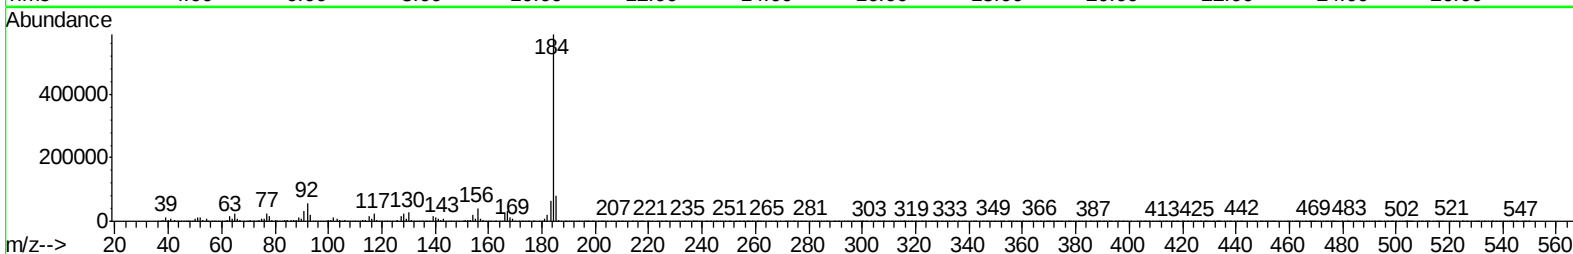


Data Path : Z:\HPCHEM1\BNA_E\Data\BE070516\
Data File : BE091968.D
Acq On : 5 Jul 2016 19:09
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 06 08:05:32 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 05 17:15:08 2016
Response via : Initial Calibration

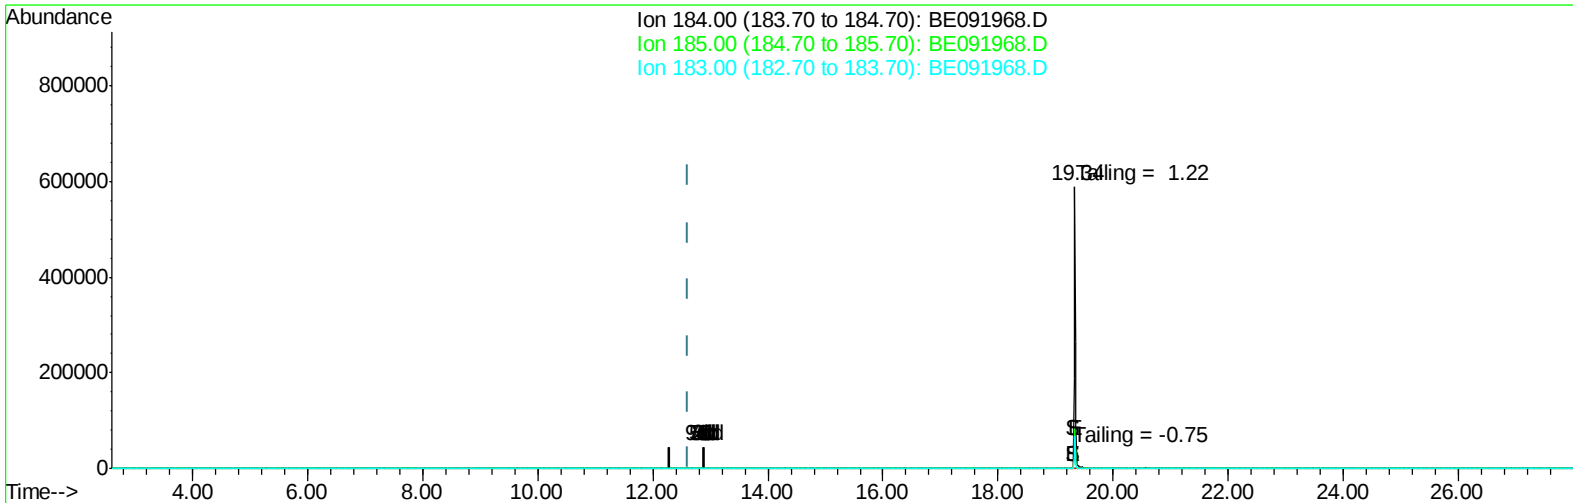

TIC: BE091968.D

(76) Benzidine




19.336min (+6.720) 497827.09ng m

response 780048

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.05
183.00	11.60	11.31
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE070516\
Data File : BE091968.D
Acq On : 5 Jul 2016 19:09
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 06 08:05:32 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 05 17:15:08 2016
Response via : Initial Calibration

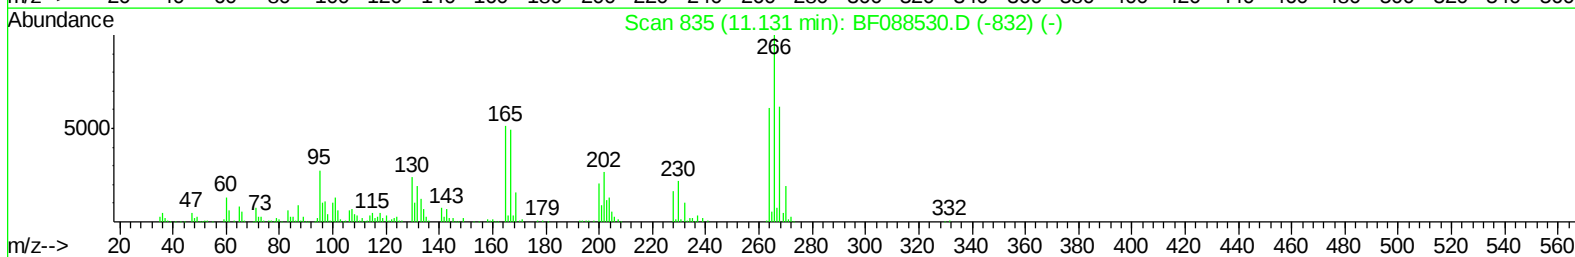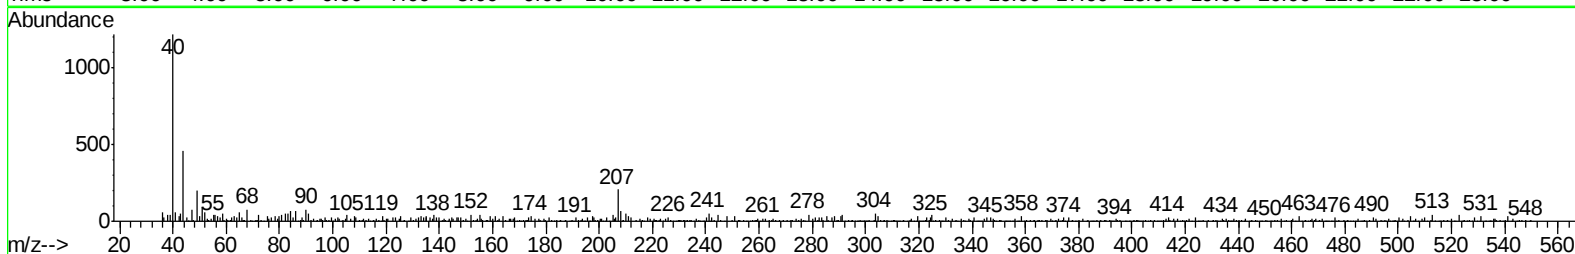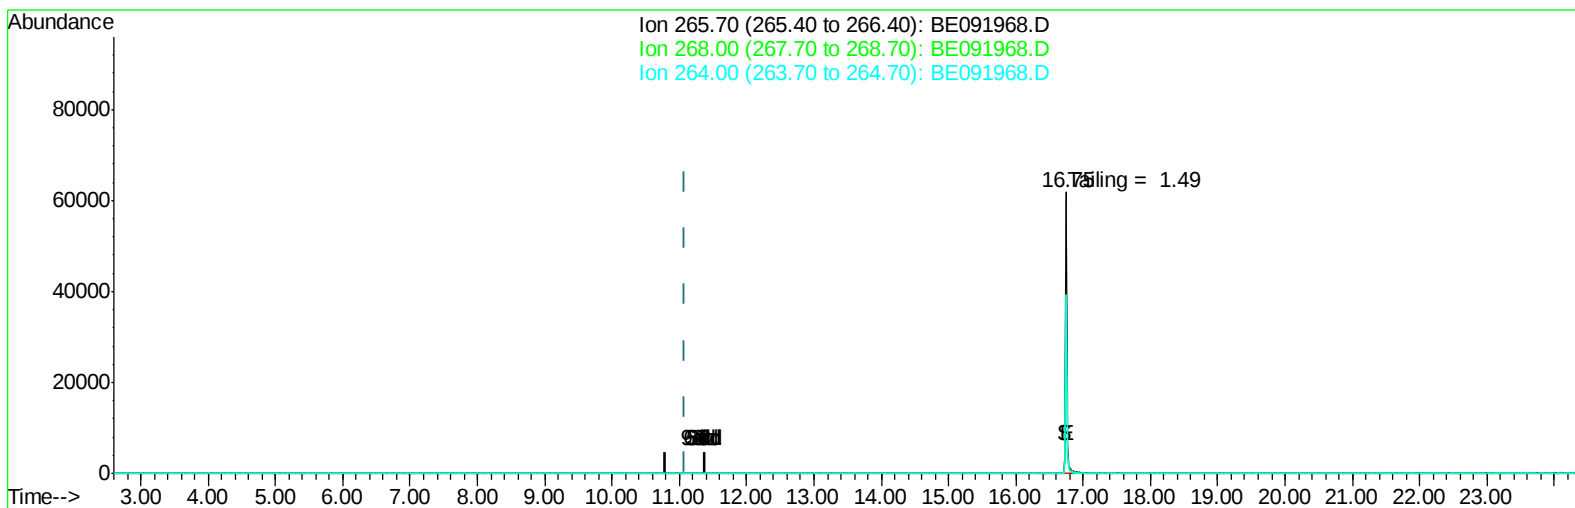

TIC: BE091968.D

(69) Pentachlorophenol (C)

11.328min (+0.232) 84.82ng

response 14

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	34.78#
264.00	62.00	34.78#
0.00	0.00	0.00