


Data Path : Z:\HPCHEM1\BNA E\DATA\BE070516\
 Data File : BE091957.D
 Acq On : 5 Jul 2016 8:15
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE070516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 05 16:14:58 2016

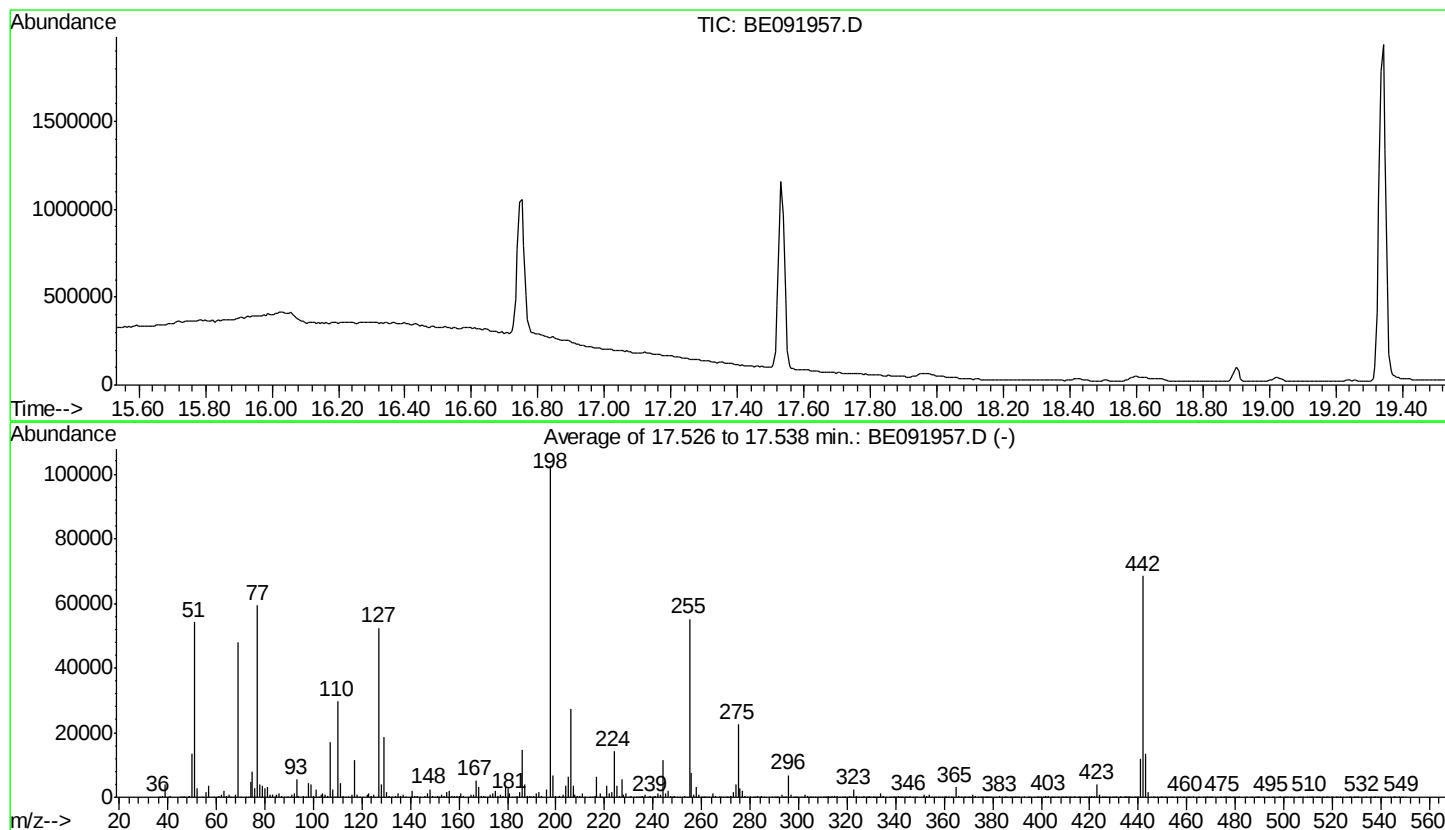

AutoFind: Scans 2542, 2543, 2544; Background Corrected with Scan 2536

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.7	54116	PASS
68	69	0.00	2	1.9	899	PASS
69	198	0.00	100	46.7	47953	PASS
70	69	0.00	2	0.1	39	PASS
127	198	10	80	51.0	52347	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	102607	PASS
199	198	5	9	6.5	6675	PASS
275	198	10	60	21.9	22517	PASS
365	198	1	100	3.0	3062	PASS
441	442	0.01	24	17.6	12023	PASS
442	198	50	100	66.6	68356	PASS
443	442	15	24	19.8	13563	PASS