
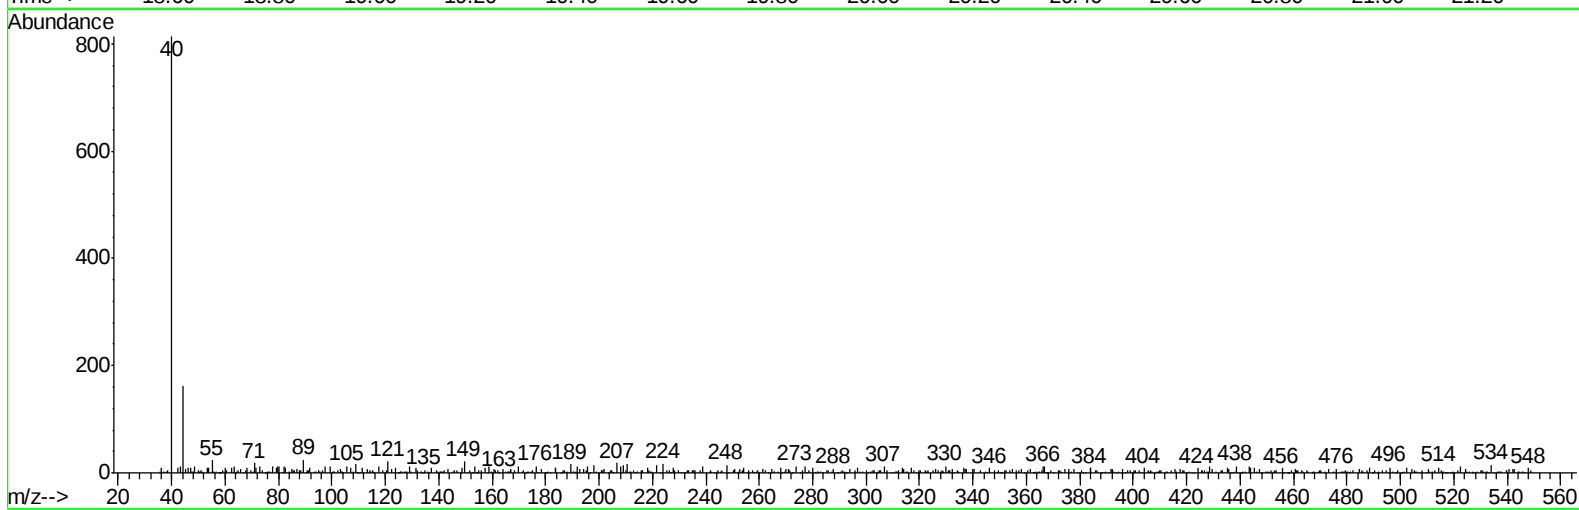


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE070519\
Data File : BE100374.D
Acq On : 5 Jul 2019 10:42
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 06 06:57:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 01:27:44 2013
Response via : Initial Calibration

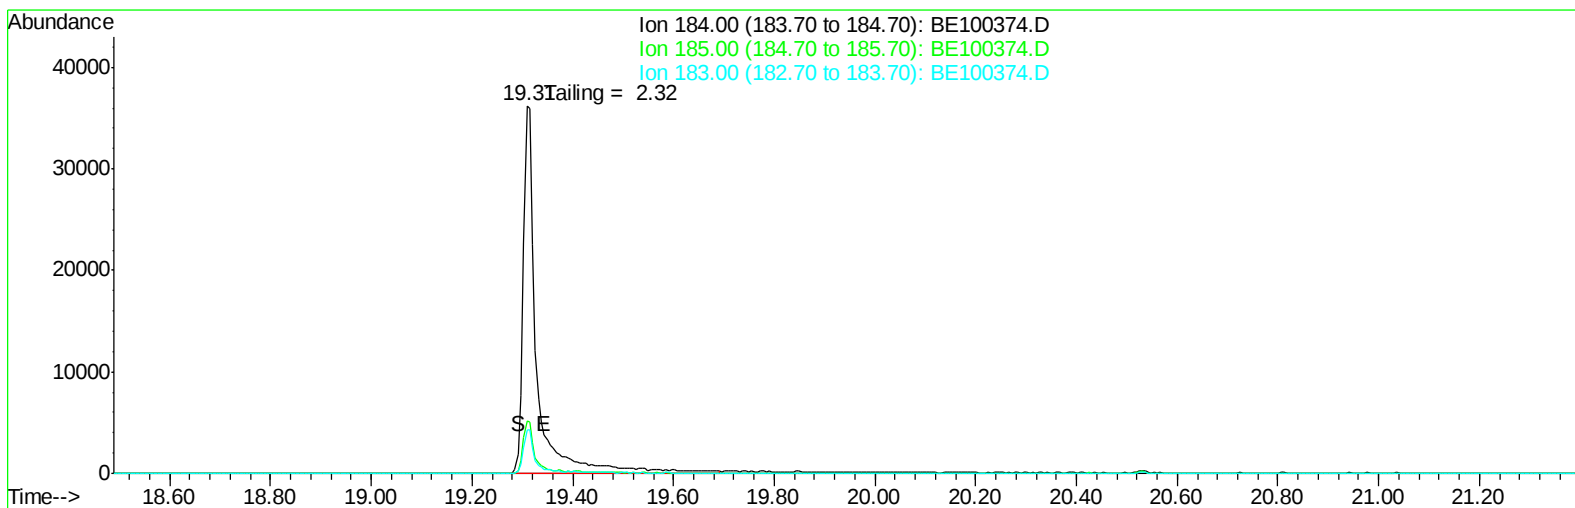

TIC: BE100374.D

(76) Benzidine



14.573min (-0.017) 98.66ng

response 10

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	0.00#
183.00	12.20	100.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE070519\
Data File : BE100374.D
Acq On : 5 Jul 2019 10:42
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 06 06:57:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 01:27:44 2013
Response via : Initial Calibration

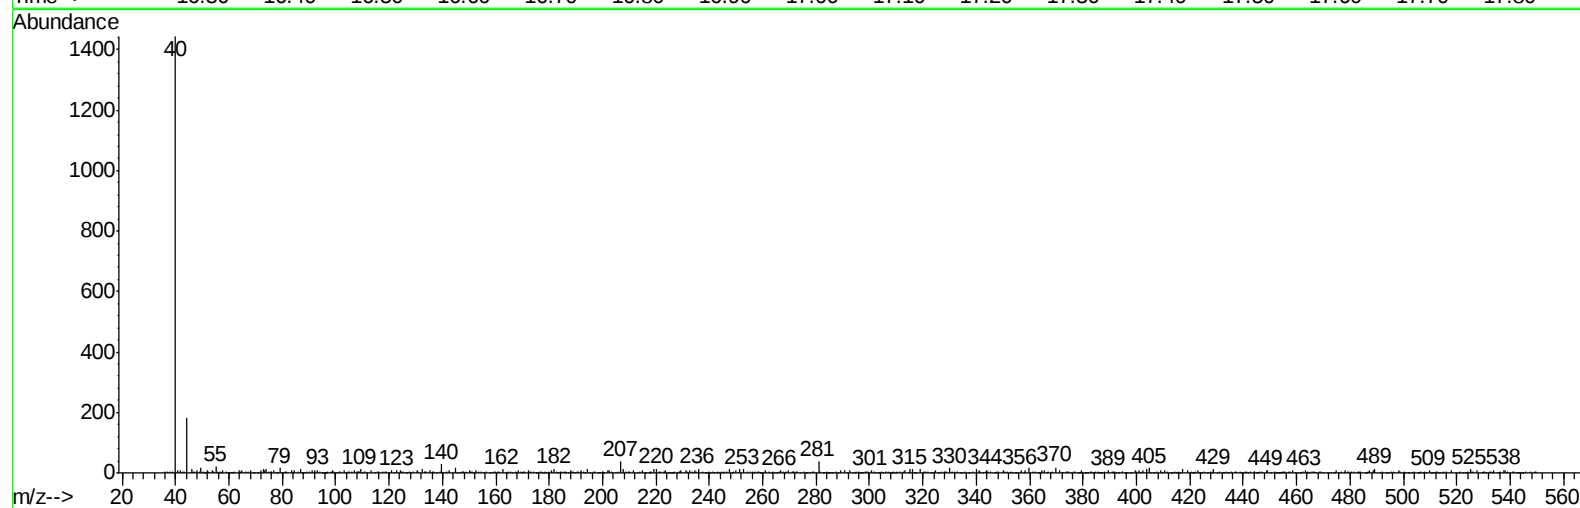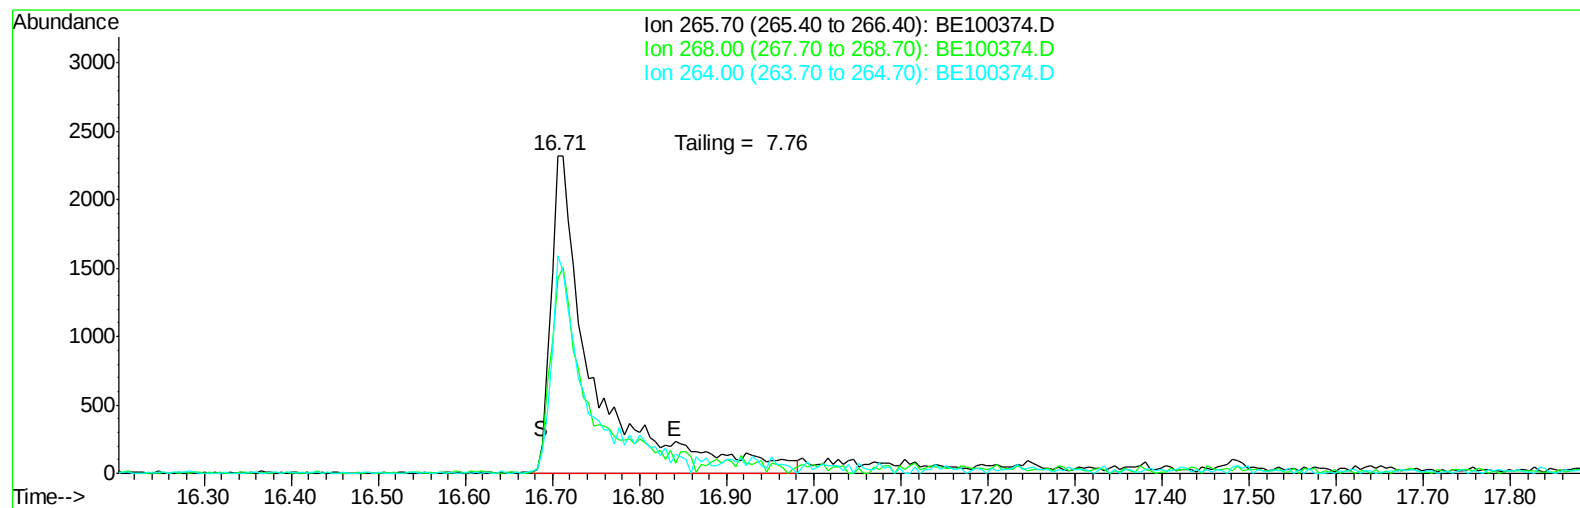

TIC: BE100374.D

(69) Pentachlorophenol (C)

12.129min (+0.041) 17.18ng

response 3

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	75.00
264.00	65.00	62.50
0.00	0.00	0.00