
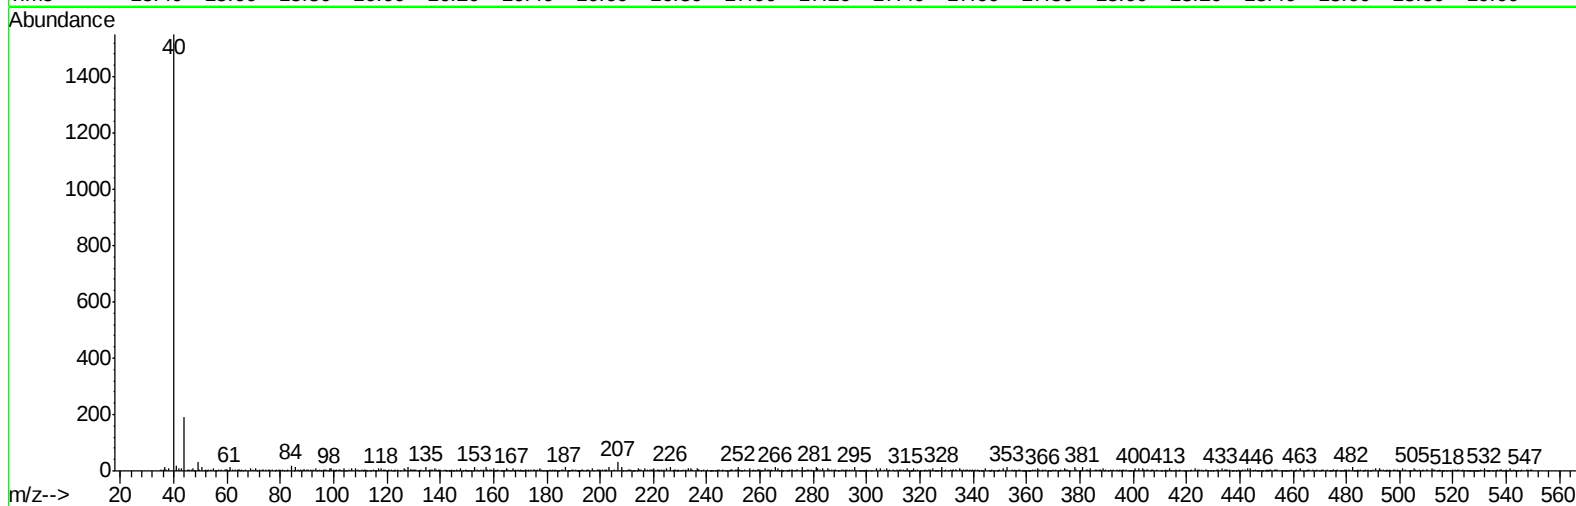


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE070519\
Data File : BE100393.D
Acq On : 5 Jul 2019 22:48
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 06 07:08:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 01:27:44 2013
Response via : Initial Calibration

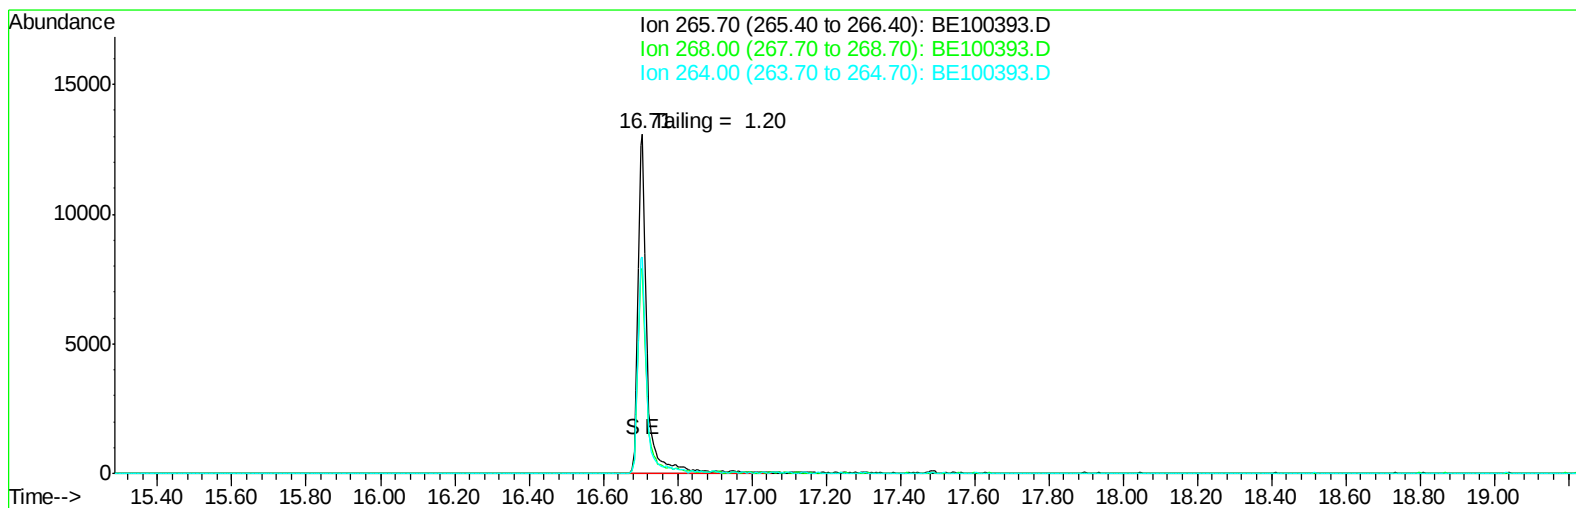

TIC: BE100393.D

(69) Pentachlorophenol (C)



12.323min (+0.236) 210.41ng

response 7

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	53.85
264.00	65.00	53.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE070519\
Data File : BE100393.D
Acq On : 5 Jul 2019 22:48
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 06 07:08:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 01:27:44 2013
Response via : Initial Calibration

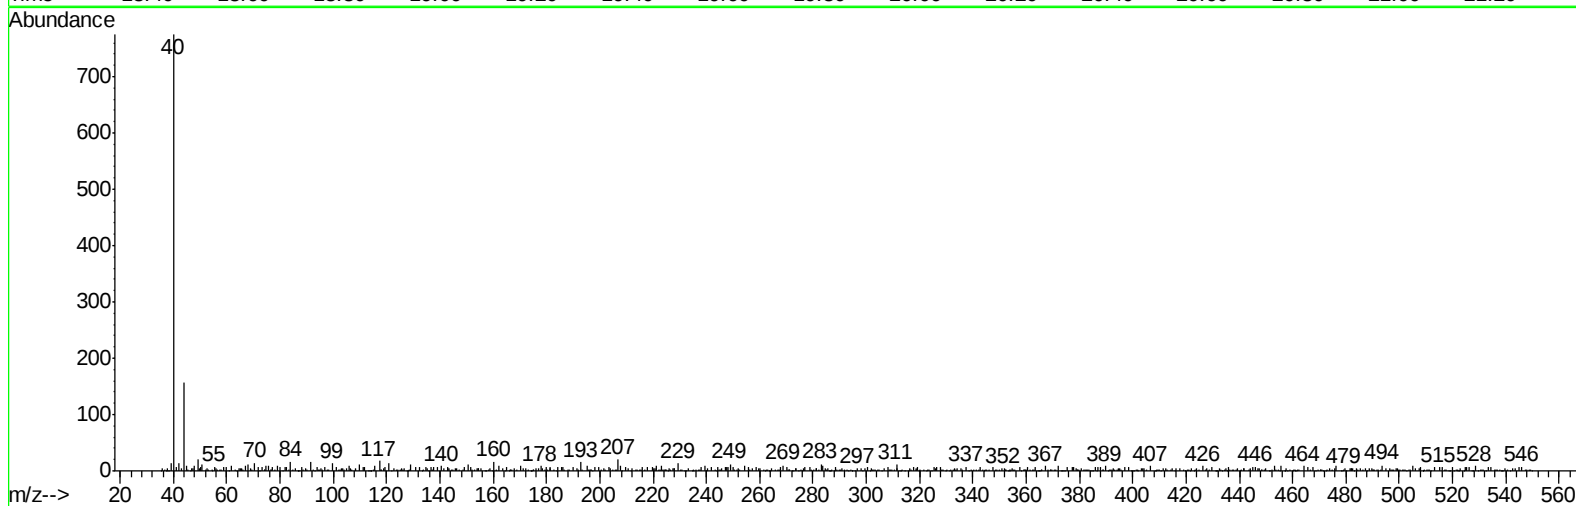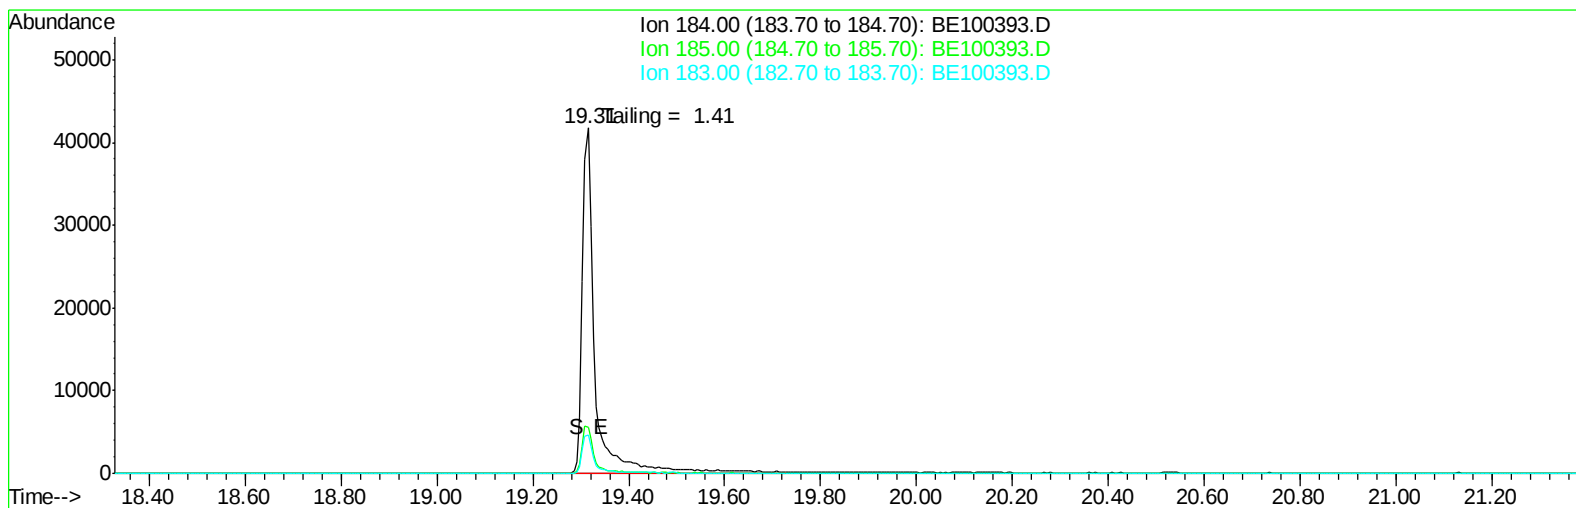

TIC: BE100393.D

(76) Benzidine

14.744min (+0.154) 24.67ng

response 4

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	100.00#
183.00	12.20	66.67#
0.00	0.00	0.00