


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070519\
Data File : BE100374.D
Acq On : 5 Jul 2019 10:42
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE062819.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 28 14:06:53 2019

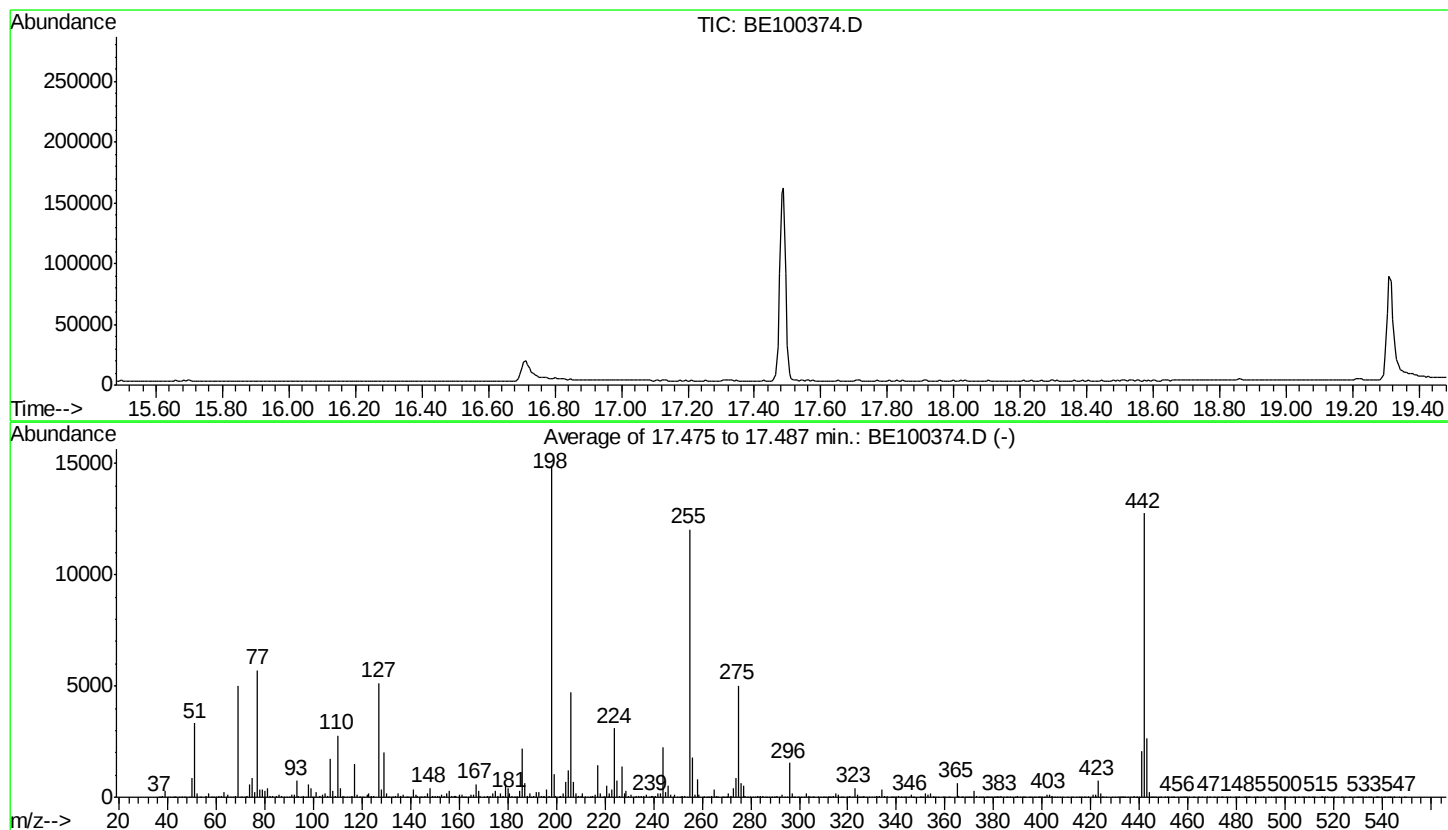

AutoFind: Scans 2534, 2535, 2536; Background Corrected with Scan 2527

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.4	3335	PASS
68	69	0.00	2	1.3	65	PASS
69	198	0.00	100	33.6	5005	PASS
70	69	0.00	2	0.4	21	PASS
127	198	10	80	34.5	5145	PASS
197	198	0.00	2	0.3	45	PASS
198	198	100	100	100.0	14912	PASS
199	198	5	9	6.9	1027	PASS
275	198	10	60	33.8	5034	PASS
365	198	1	100	4.4	651	PASS
441	198	0.01	100	14.1	2099	PASS
442	198	50	100	85.5	12755	PASS
443	442	15	24	20.6	2630	PASS