


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE070519\
Data File : BE100393.D
Acq On : 5 Jul 2019 22:48
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE062819.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 28 14:06:53 2019

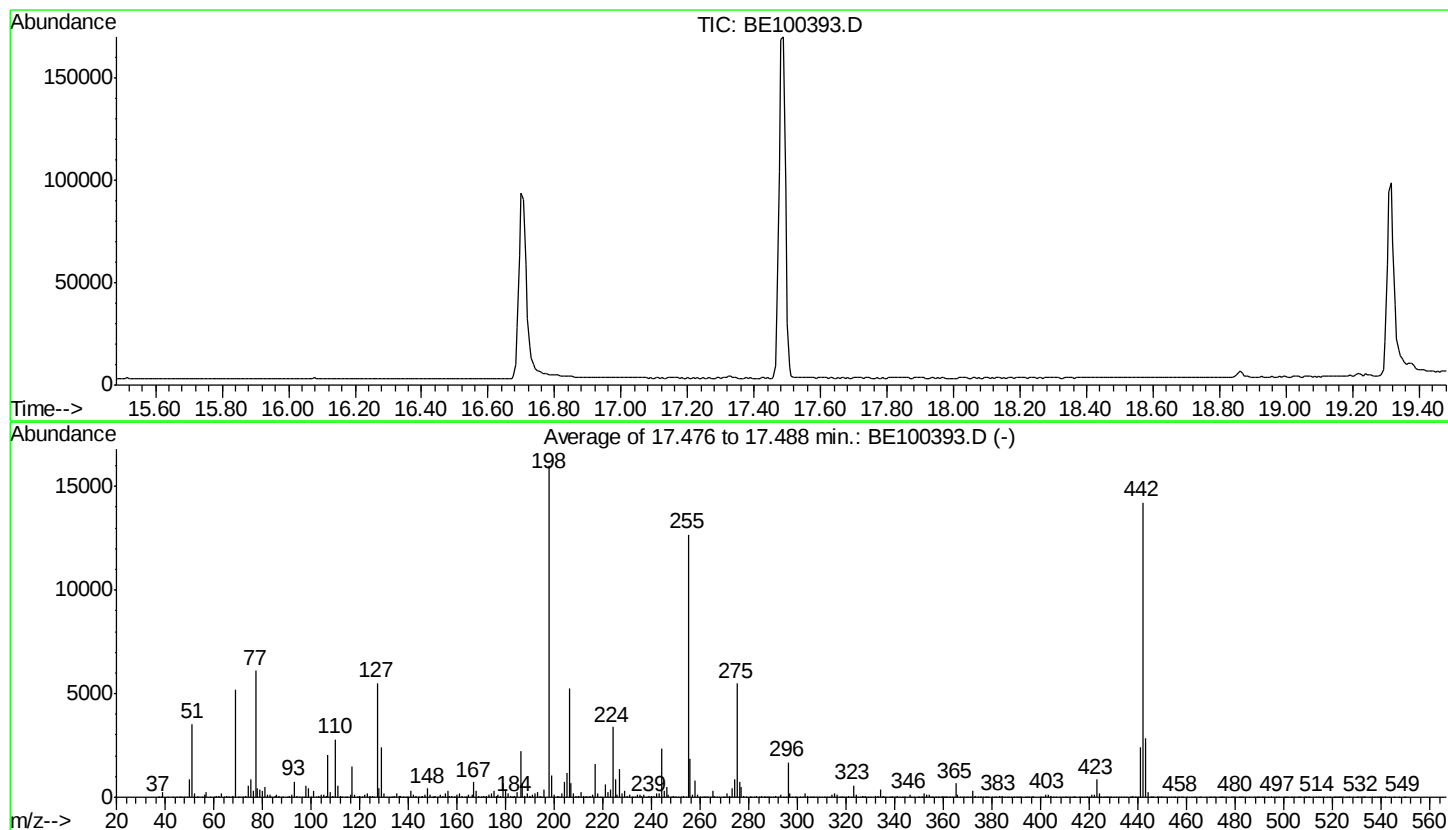

AutoFind: Scans 2534, 2535, 2536; Background Corrected with Scan 2526

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.1	3541	PASS
68	69	0.00	2	0.8	43	PASS
69	198	0.00	100	32.5	5202	PASS
70	69	0.00	2	0.6	32	PASS
127	198	10	80	34.4	5501	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	16007	PASS
199	198	5	9	6.7	1078	PASS
275	198	10	60	34.3	5494	PASS
365	198	1	100	4.1	651	PASS
441	198	0.01	100	15.1	2415	PASS
442	198	50	100	88.8	14217	PASS
443	442	15	24	20.0	2850	PASS