


Data Path : Z:\HPCHEM1\BNA_E\Data\BE070615\
Data File : BE090055.D
Acq On : 6 Jul 2015 14:19
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BE062915.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 30 07:01:01 2015

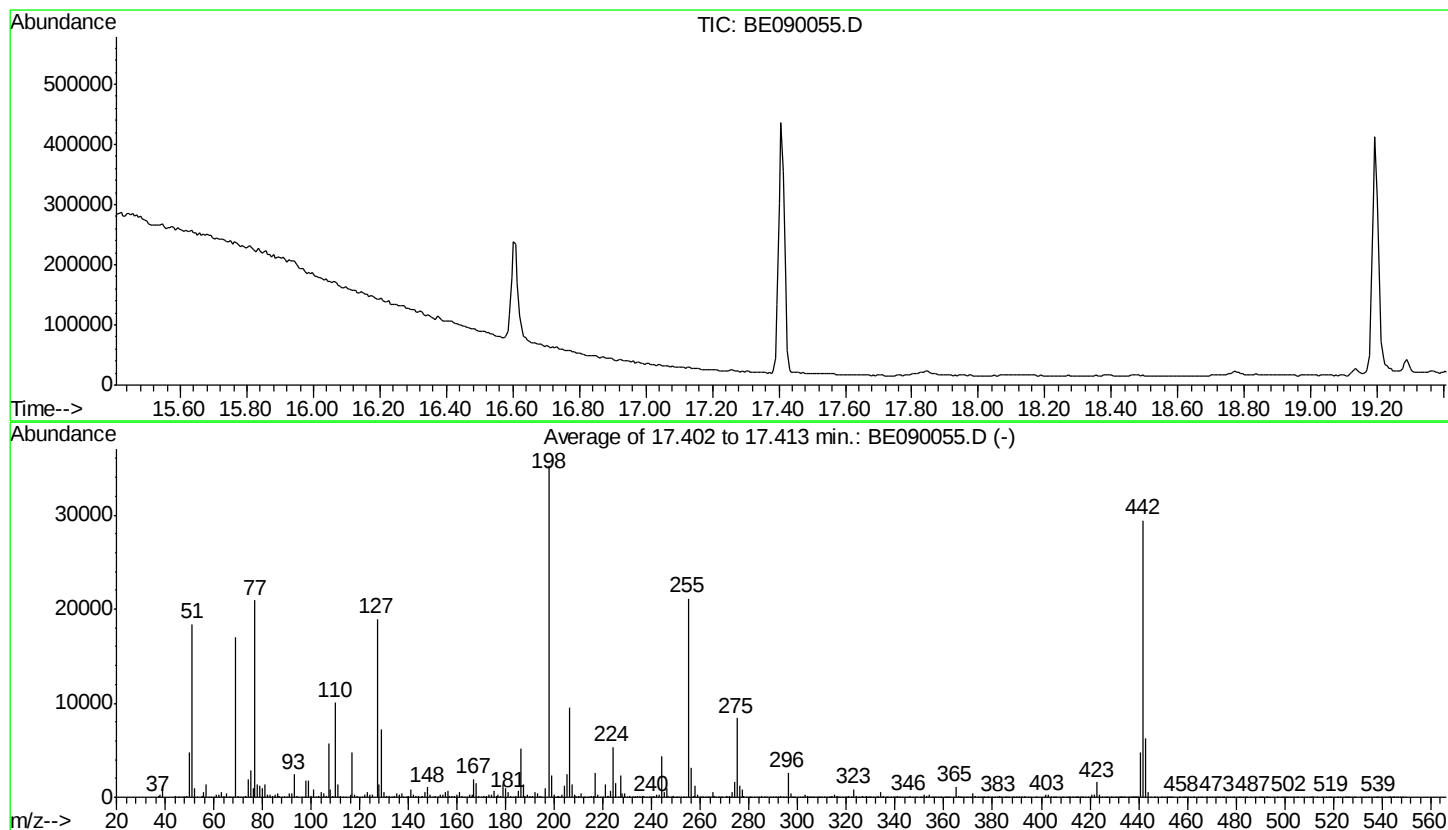

AutoFind: Scans 2521, 2522, 2523; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.3	18423	PASS
68	69	0.00	2	0.2	41	PASS
69	198	0.00	100	48.3	17039	PASS
70	69	0.00	2	0.7	126	PASS
127	198	10	80	53.8	18976	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	35242	PASS
199	198	5	9	6.8	2384	PASS
275	198	10	60	23.9	8410	PASS
365	198	1	100	3.2	1119	PASS
441	442	0.01	24	16.4	4814	PASS
442	198	50	100	83.4	29394	PASS
443	442	15	24	21.3	6274	PASS