
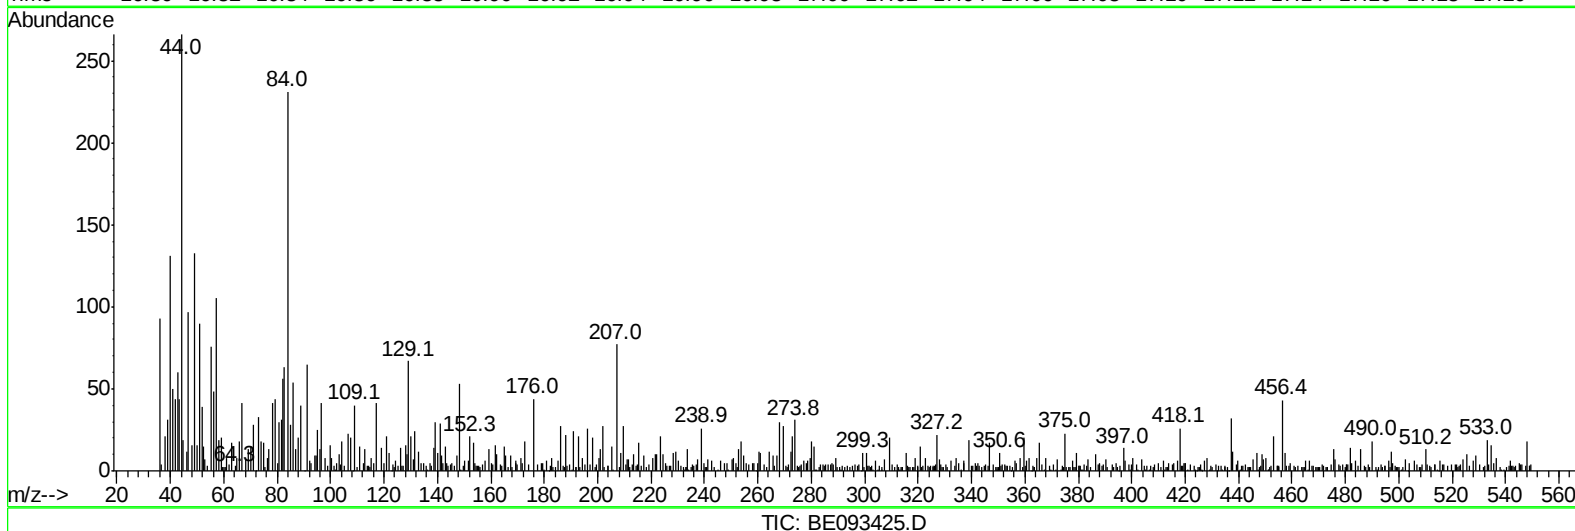


Data Path : Z:\HPCHEM1\BNA E\DATA\BE070617\
Data File : BE093425.D
Acq On : 6 Jul 2017 8:48
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jul 07 07:25:40 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF070117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 05 13:27:10 2017
Response via : Initial Calibration

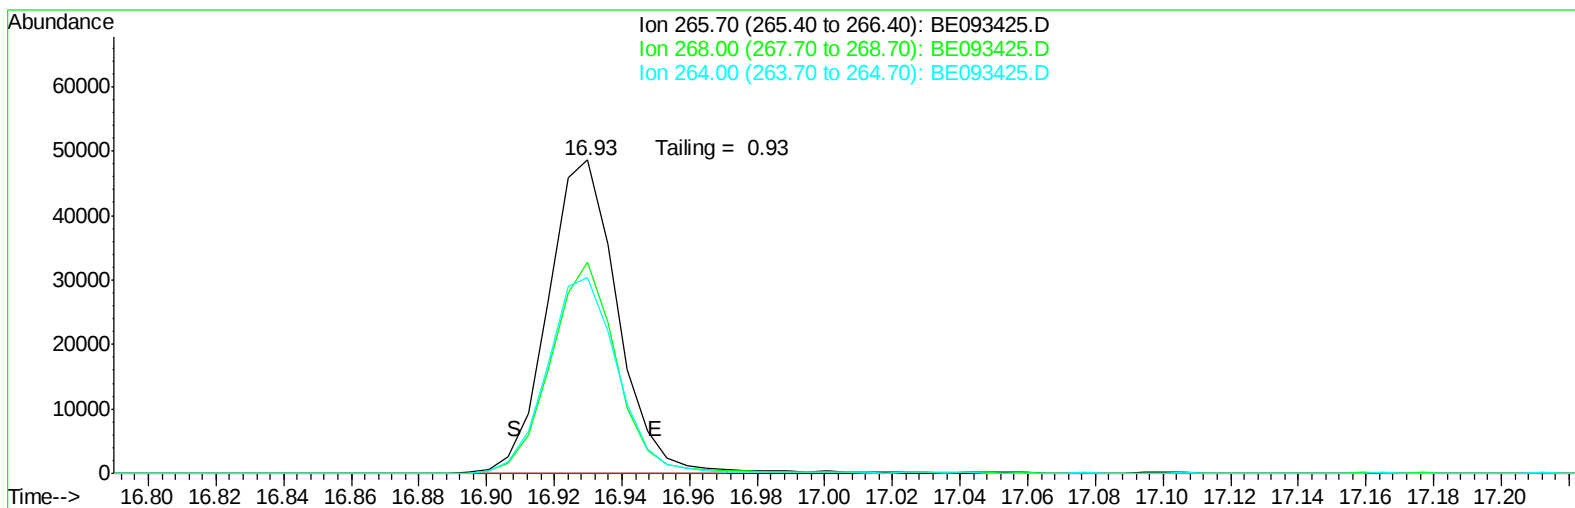

(69) Pentachlorophenol (C)

10.990min (-0.049) 71.25ng

response 9

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	250.00#
264.00	64.60	100.00#
0.00	0.00	0.00