


Data Path : Z:\HPCHEM1\BNA_E\Data\BE070617\
 Data File : BE093425.D
 Acq On : 6 Jul 2017 8:48
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE070217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 03 06:40:23 2017

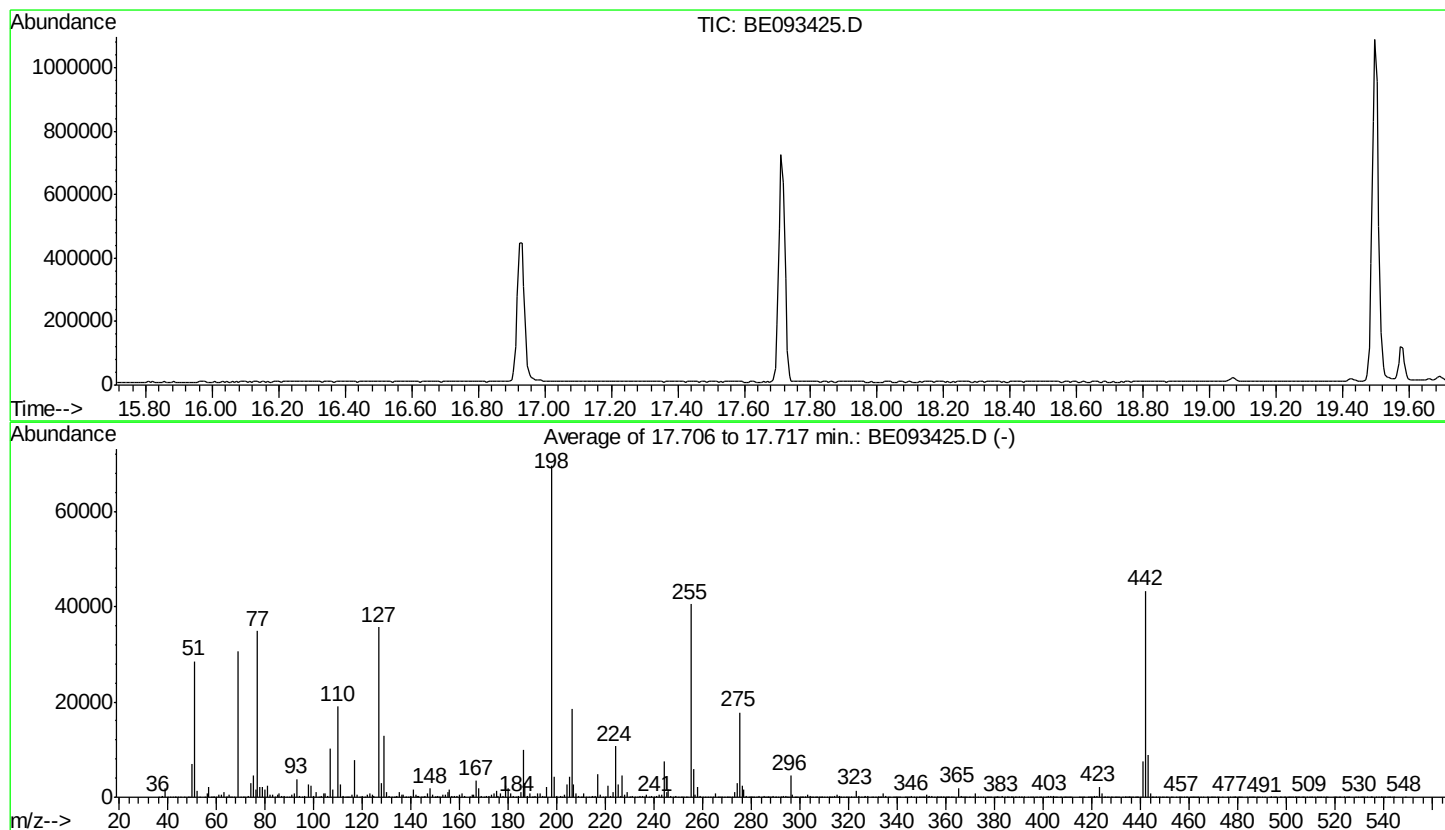

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2562

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	28533	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	44.1	30725	PASS
70	69	0.00	2	0.5	141	PASS
127	198	10	80	51.3	35701	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	69597	PASS
199	198	5	9	6.4	4420	PASS
275	198	10	60	25.6	17788	PASS
365	198	1	100	2.8	1979	PASS
441	442	0.01	24	17.1	7421	PASS
442	198	50	100	62.3	43387	PASS
443	442	15	24	20.2	8779	PASS