
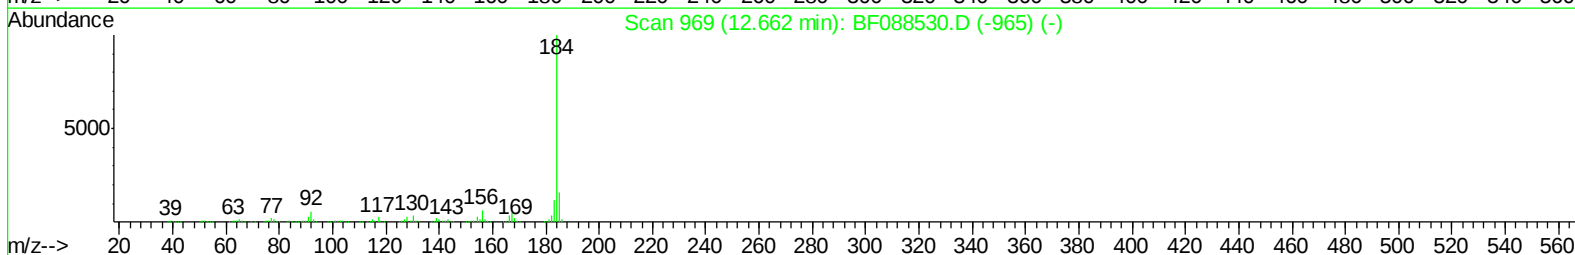
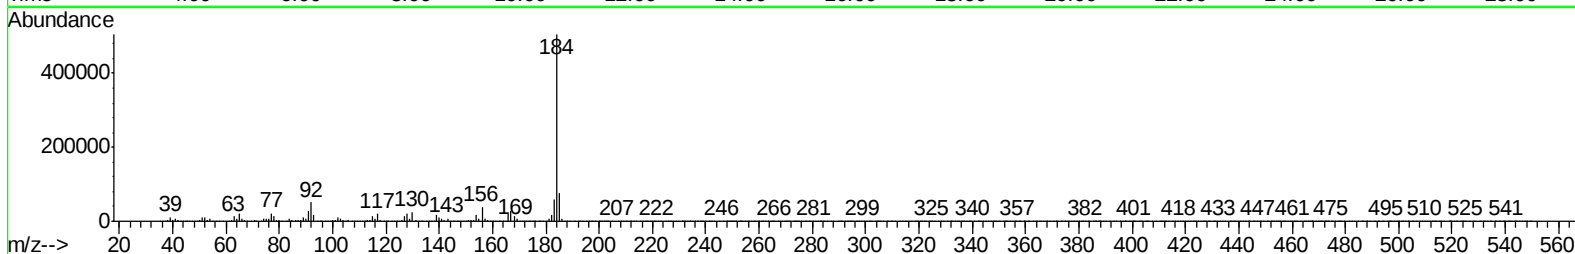


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE070716\
Data File : BE091983.D
Acq On : 7 Jul 2016 16:33
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 07:14:08 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 05 17:15:08 2016
Response via : Initial Calibration

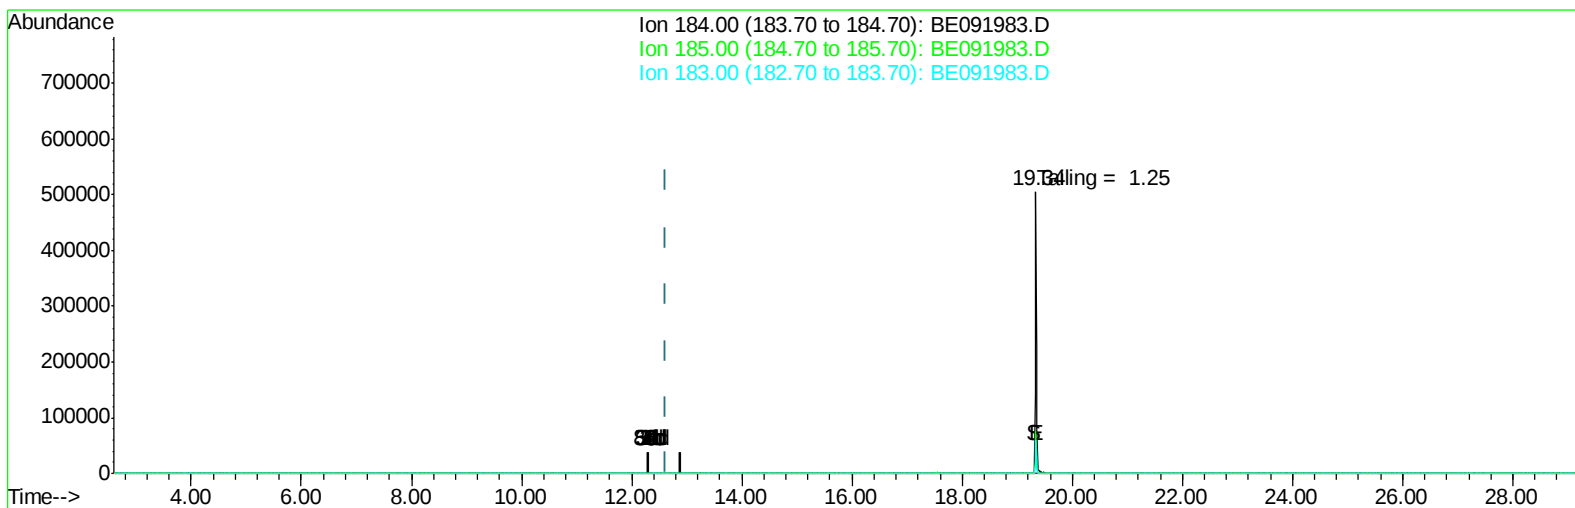

TIC: BE091983.D

(76) Benzidine




19.341min (+6.724) 345001.88ng m

response 662653

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.97
183.00	11.60	11.64
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE070716\
Data File : BE091983.D
Acq On : 7 Jul 2016 16:33
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 07:14:08 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 05 17:15:08 2016
Response via : Initial Calibration

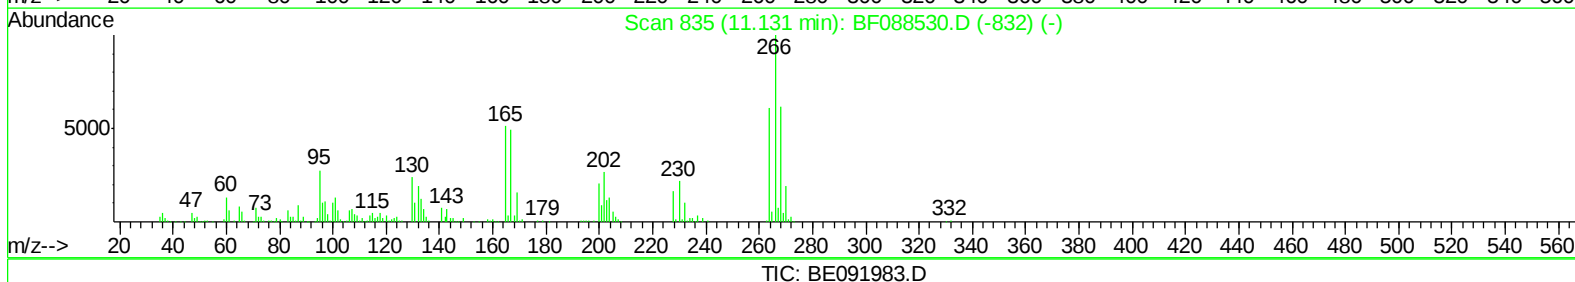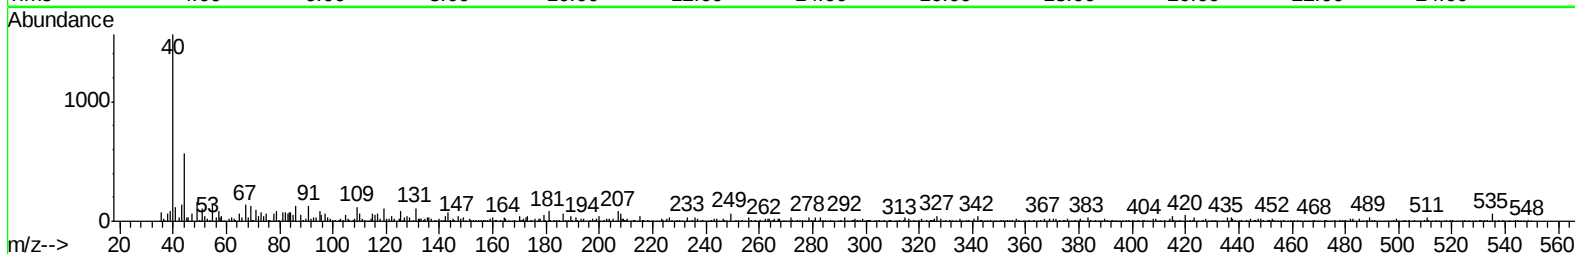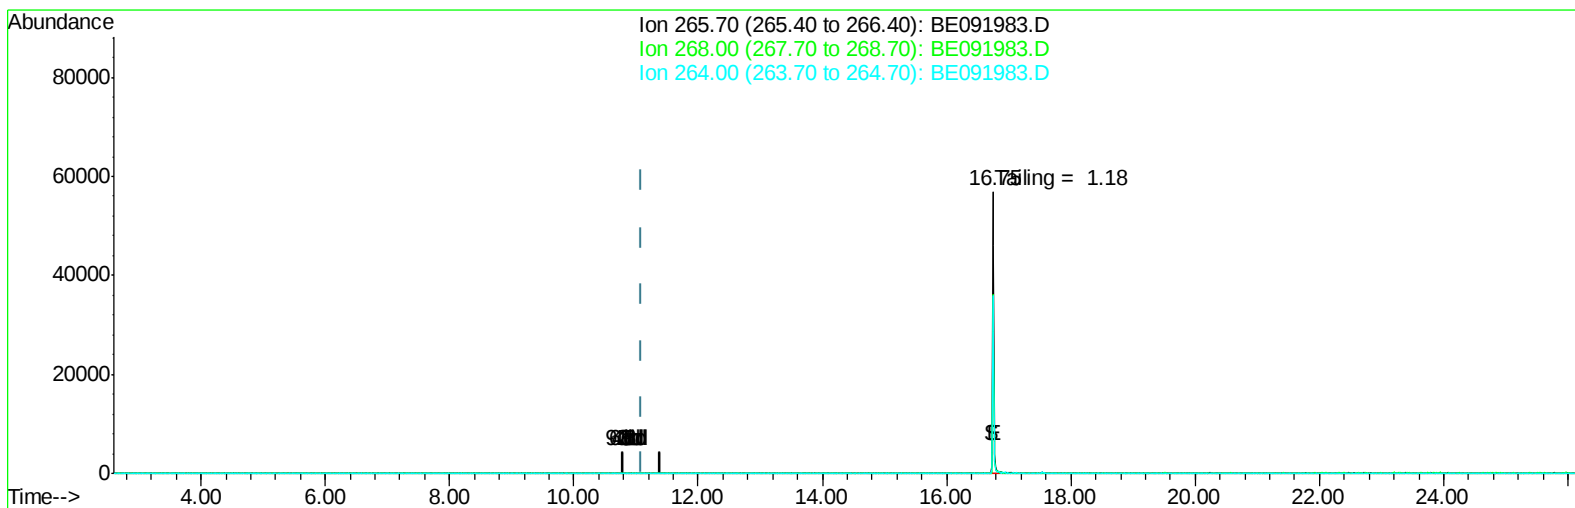

TIC: BE091983.D

(69) Pentachlorophenol (C)
10.845min (-0.251) 132.54ng
response 35

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	108.33#
264.00	62.00	83.33#
0.00	0.00	0.00