

Data Path : Z:\HPCHEM1\BNA E\DATA\BE070716\
 Data File : BE091986.D
 Acq On : 7 Jul 2016 18:23
 Operator : UM/SJ
 Sample : H3697-03
 Misc : 4X internal std added
 ALS Vial : 4 Sample Multiplier: 4

Instrument :
 BNA_E
 ClientSampleId :
 FB-06202016

Quant Time: Jul 08 16:12:32 2016
 Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE070516.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 05 16:14:58 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.20	152	125332	20.00	ng	0.00
8) Naphthalene-d8	10.99	136	577370	20.00	ng	0.00
15) Acenaphthene-d10	14.86	164	387252	20.00	ng	0.00
24) Phenanthrene-d10	17.59	188	781312	20.00	ng	0.00
31) Chrysene-d12	21.76	240	1127749	20.00	ng	0.00
40) Perylene-d12	24.17	264	1034865	20.00	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.72	112	528340	70.49	ng	0.00
5) Phenol-d6	7.35	99	444447	42.68	ng	-0.02
9) Nitrobenzene-d5	9.37	82	1040596	105.85	ng	-0.02
16) 2,4,6-Tribromophenol	16.35	330	414375	117.94	ng	0.00
17) 2-Fluorobiphenyl	13.49	172	1868707	79.12	ng	0.00
34) Terphenyl-d14	20.22	244	2469356	74.26	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA E\DATA\BE070716\
Data File : BE091986.D
Acq On : 7 Jul 2016 18:23
Operator : UM/SJ
Sample : H3697-03
Misc : 4X internal std added
ALS Vial : 4 Sample Multiplier: 4

Instrument :
BNA_E
ClientSampleId :
FB-06202016

Quant Time: Jul 08 16:12:32 2016
Quant Method : Z:\HPCHEM1\BNA E\METHODS\8270-SIM-BE070516.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 05 16:14:58 2016
Response via : Initial Calibration

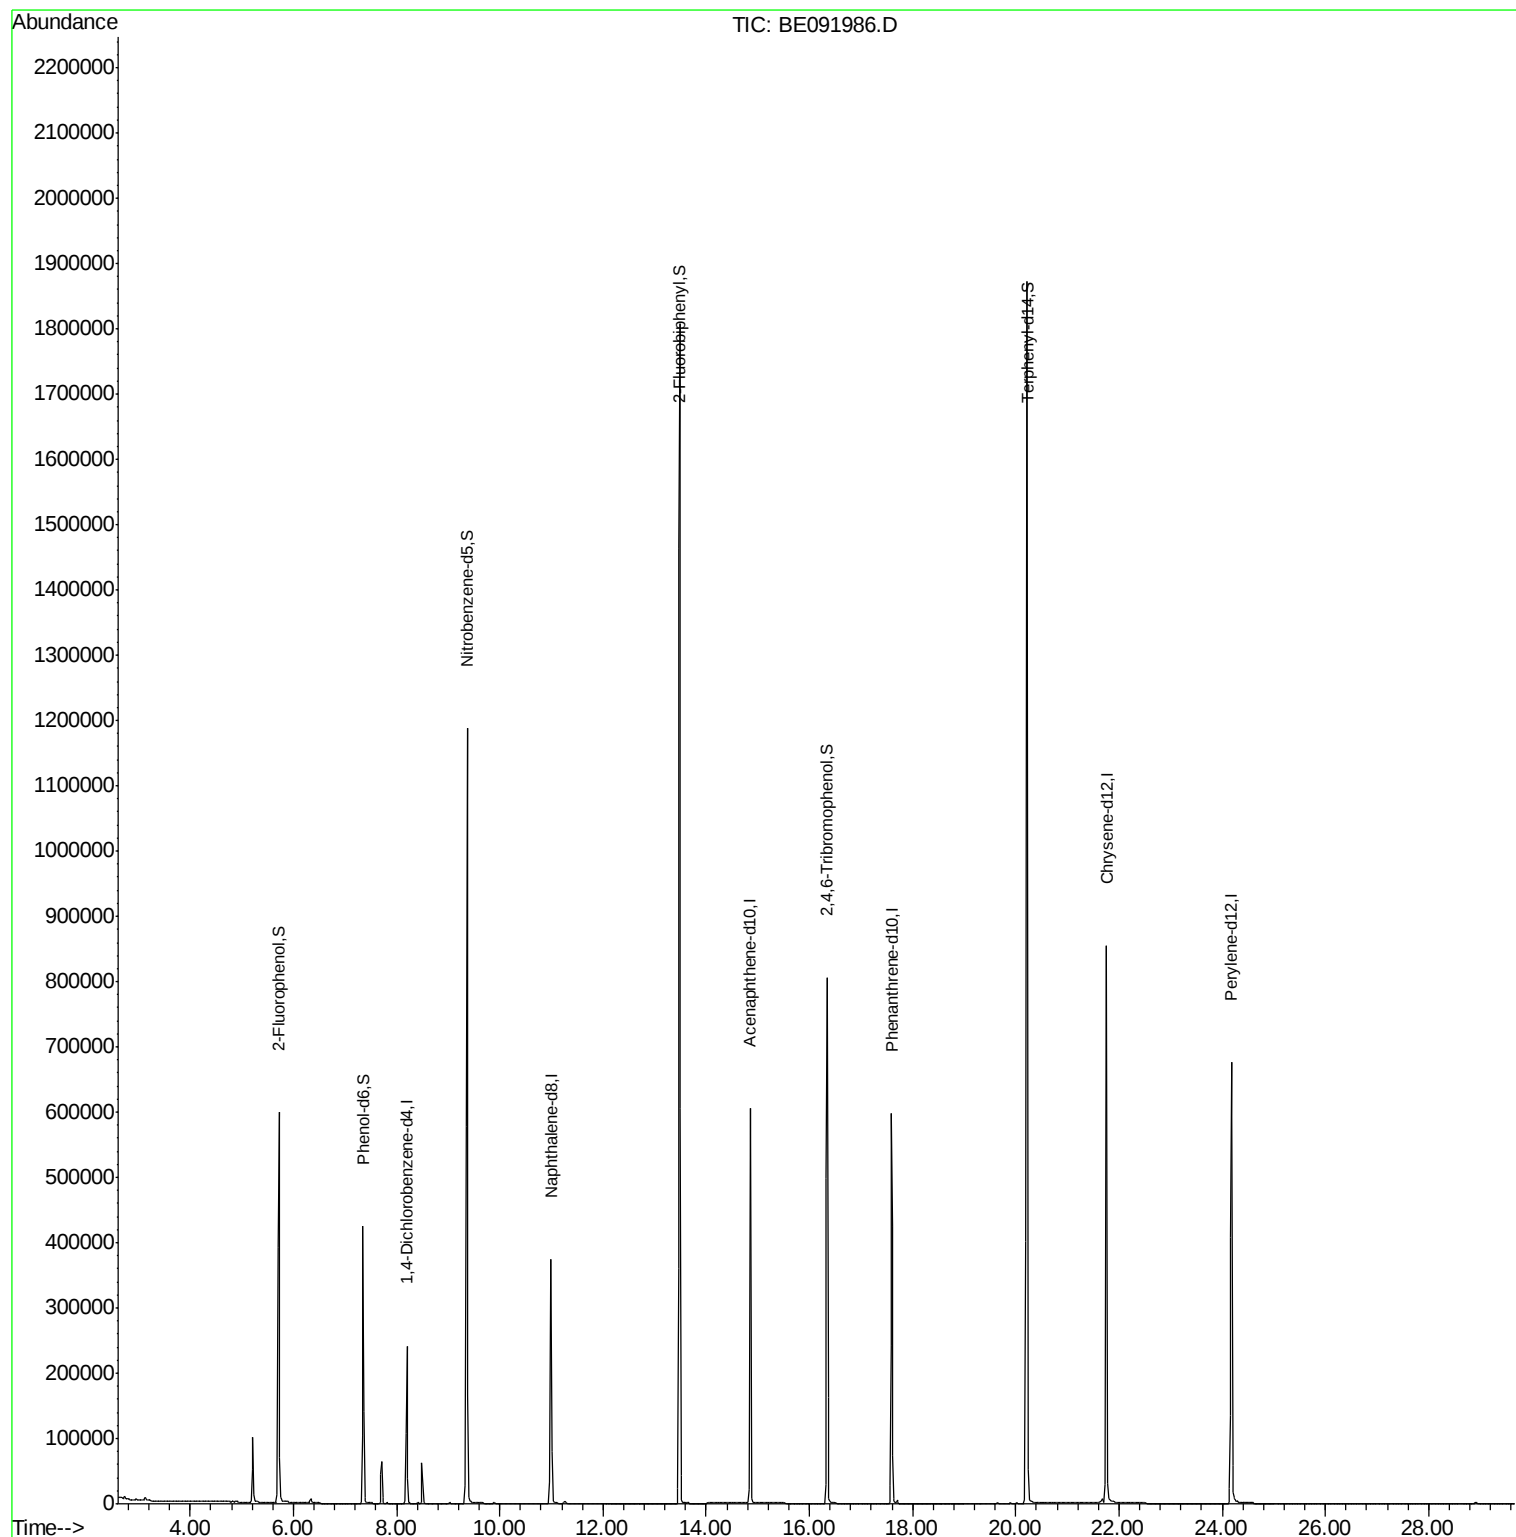




#1


1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.20 min Scan# 323
Delta R.T. 0.00 min
Lab File: BE091986.D
Acq: 7 Jul 2016 18:23

Instrument :
BNA_E
ClientSampleId :
FB-06202016



Tot Ion:152 Resp: 125332
Ion Ratio Lower Upper
152 100
150 150.0 123.9 185.9
115 55.7 48.3 72.5

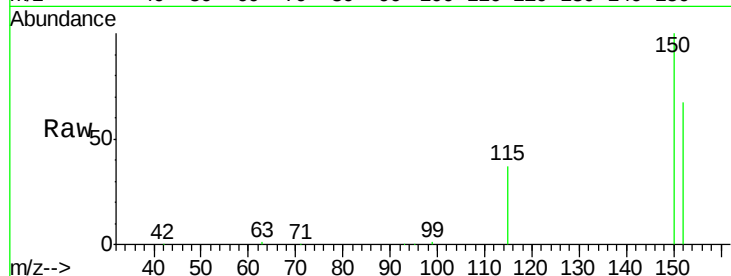

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

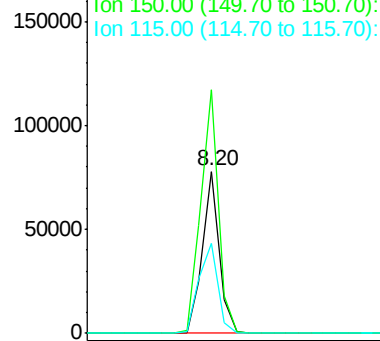


Time-->

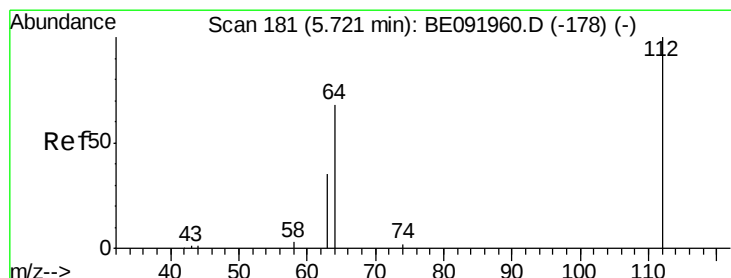


#4

2-Fluorophenol
Concen: 70.49 ng
RT: 5.72 min Scan# 181
Delta R.T. -0.00 min
Lab File: BE091986.D
Acq: 7 Jul 2016 18:23


Tgt Ion:112 Resp: 528340
Ion Ratio Lower Upper
112 100
64 68.5 53.7 80.5
63 36.8 29.5 44.3

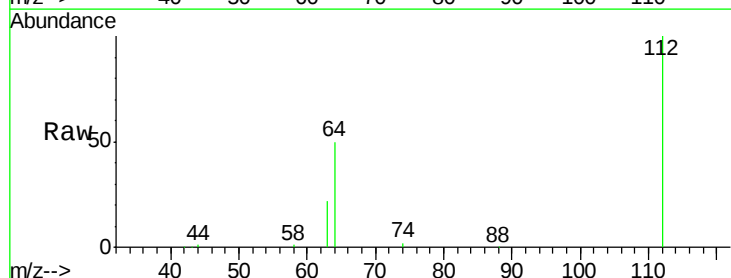


Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BE0
Ion 63.00 (62.70 to 63.70): BE0

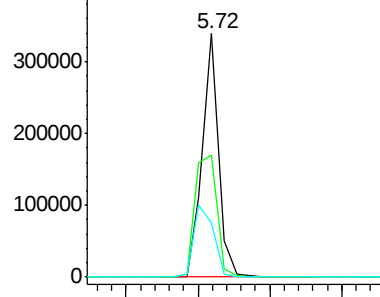

Time-->





#5

Phenol-d6

Concen: 42.68 ng

RT: 7.35 min Scan# 274

Delta R.T. -0.02 min

Lab File: BE091986.D

Acq: 7 Jul 2016 18:23

Instrument :

BNA_E

ClientSampleId :

FB-06202016


Tot Ion: 99 Resp: 444447

Ion Ratio Lower Upper

99 100

42 24.7 19.6 29.4




71 35.9 28.1 42.1

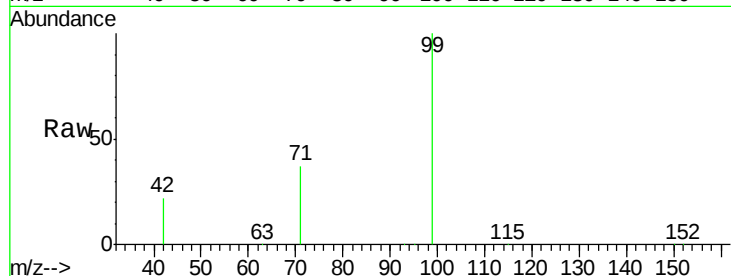

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

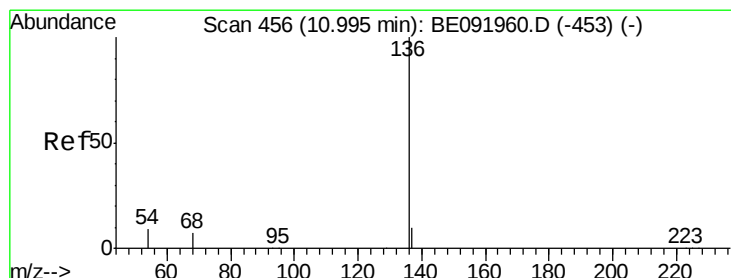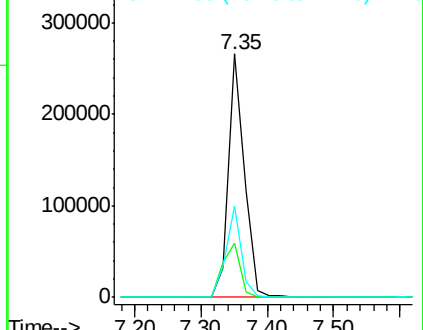

#8

Naphthalene-d8

Concen: 20.00 ng

RT: 10.99 min Scan# 456

Delta R.T. -0.00 min

Lab File: BE091986.D

Acq: 7 Jul 2016 18:23

Tgt Ion: 136 Resp: 577370


Ion Ratio Lower Upper

136 100

137 10.4 8.3 12.5

54 7.2 8.2 12.4#

68 5.5 5.9 8.9#


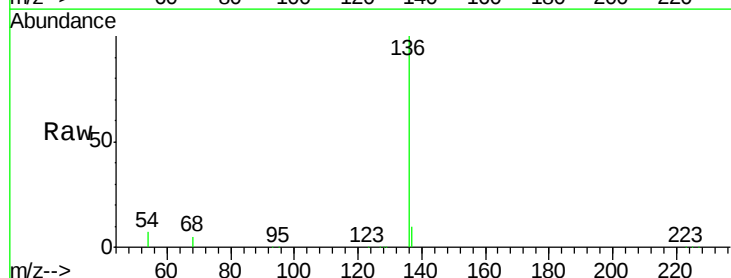



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

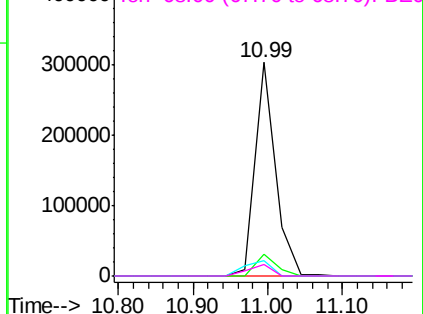

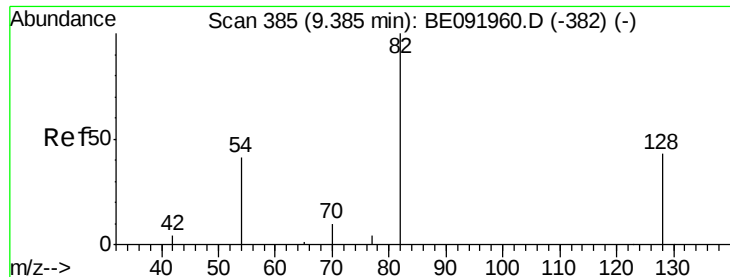

#9

Nitrobenzene-d5

Concen: 105.85 ng

RT: 9.37 min Scan# 384

Delta R.T. -0.02 min

Lab File: BE091986.D

Acq: 7 Jul 2016 18:23

Instrument :

BNA_E

ClientSampleId :

FB-06202016


Tot Ion: 82 Resp: 1040596

Ion Ratio Lower Upper




82 100

128 36.2 39.5 59.3#

54 39.5 30.3 45.5

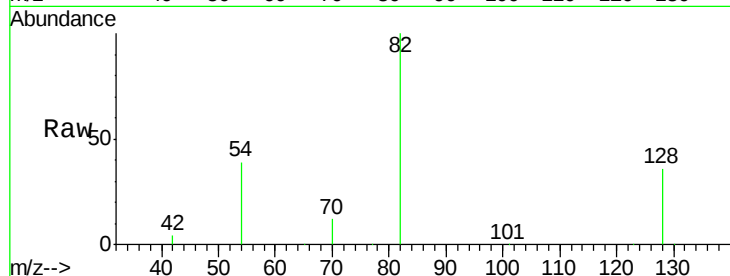

Abundance Ion 82.00 (81.70 to 82.70): BE0
Ion 128.00 (127.70 to 128.70): BE0
Ion 54.00 (53.70 to 54.70): BE0

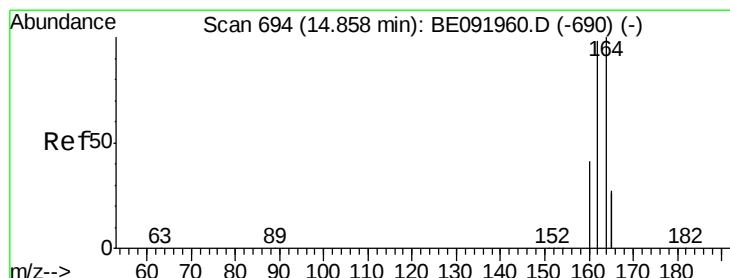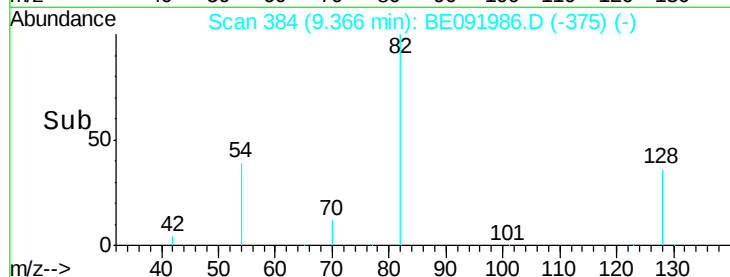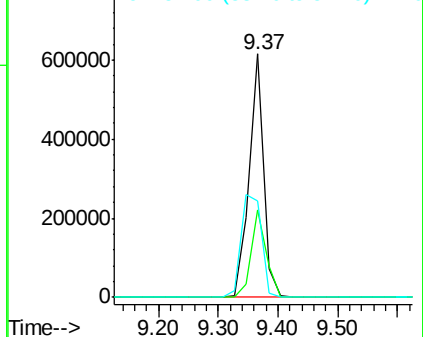

#15

Acenaphthene-d10

Concen: 20.00 ng

RT: 14.86 min Scan# 694

Delta R.T. 0.00 min

Lab File: BE091986.D

Acq: 7 Jul 2016 18:23


Tgt Ion:164 Resp: 387252

Ion Ratio Lower Upper



164 100


162 96.6 71.8 107.8

160 40.3 28.0 42.0

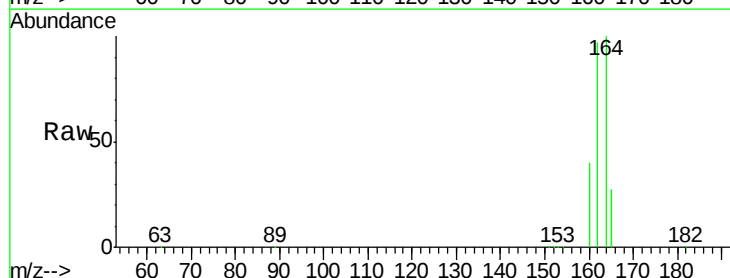

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

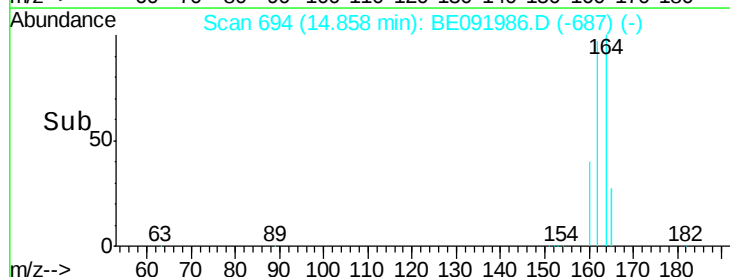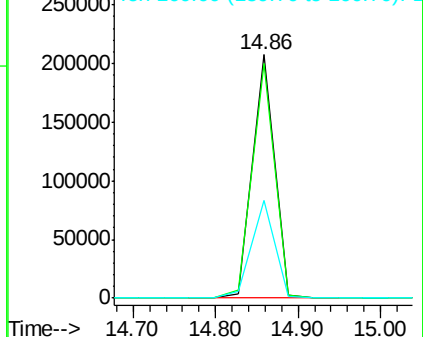


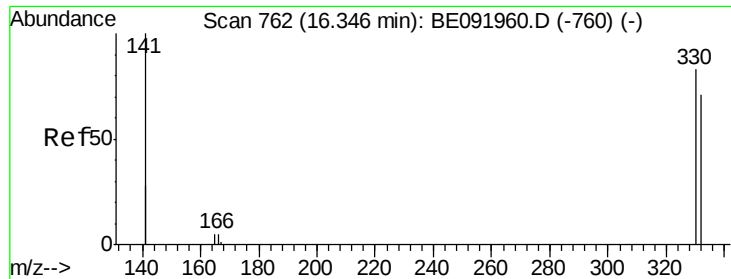




#16
 2,4,6-Tribromophenol
 Concen: 117.94 ng
 RT: 16.35 min Scan# 762
 Delta R.T. 0.00 min
 Lab File: BE091986.D
 Acq: 7 Jul 2016 18:23

Instrument :
 BNA_E
 ClientSampleId :
 FB-06202016

Tot Ion:330 Resp: 414375
 Ion Ratio Lower Upper
 330 100
 332 95.8 77.0 115.6
 141 169.0 138.4 207.6

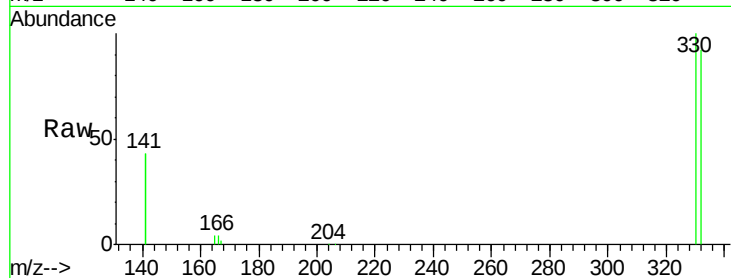


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

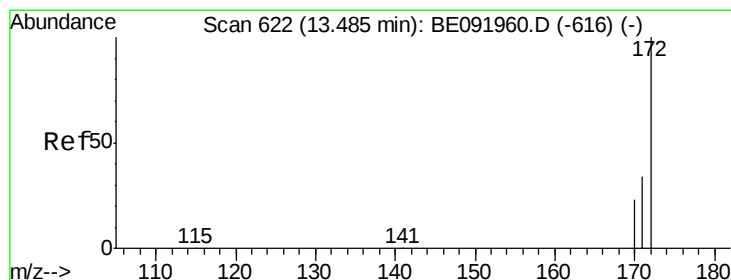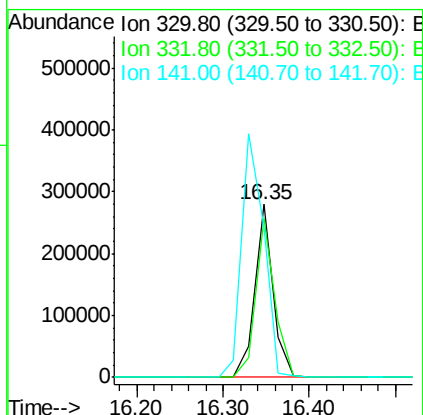




#17
 2-Fluorobiphenyl
 Concen: 79.12 ng
 RT: 13.49 min Scan# 622
 Delta R.T. 0.00 min
 Lab File: BE091986.D
 Acq: 7 Jul 2016 18:23

Tgt Ion:172 Resp: 1868707
 Ion Ratio Lower Upper
 172 100
 171 33.4 24.3 36.5
 170 20.6 14.9 22.3

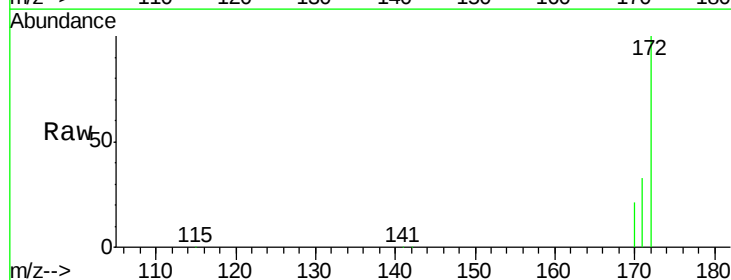

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



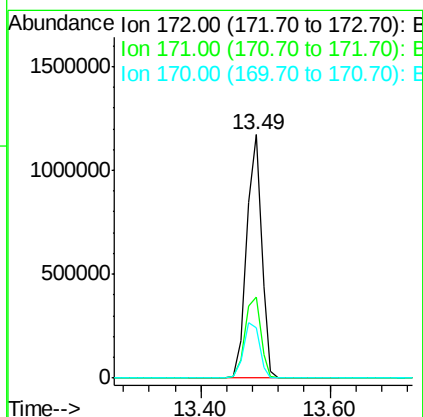
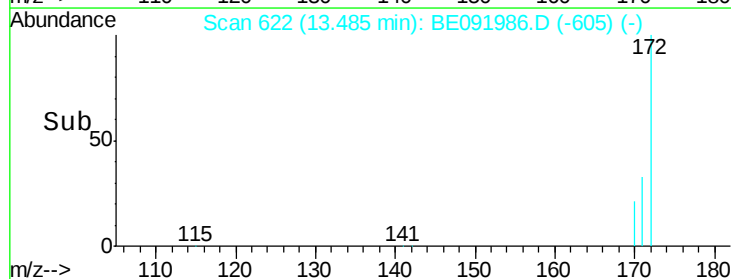




#24
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.59 min Scan# 835
Delta R.T. 0.00 min
Lab File: BE091986.D
Acq: 7 Jul 2016 18:23




Instrument :
BNA_E
ClientSampleId :
FB-06202016


Tot Ion:188 Resp: 781312
Ion Ratio Lower Upper
188 100
94 11.1 4.1 6.1#
80 11.0 3.4 5.2#

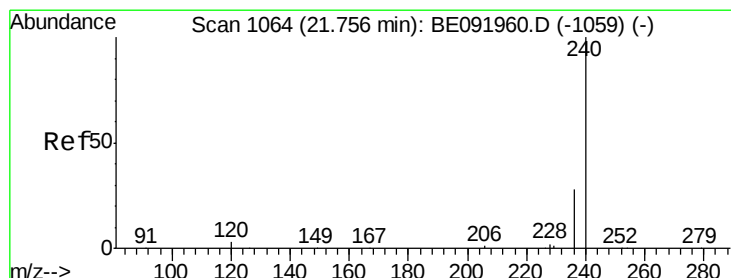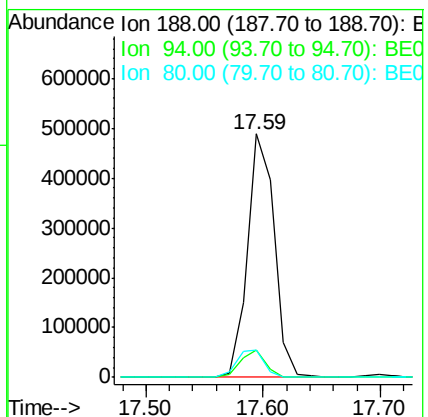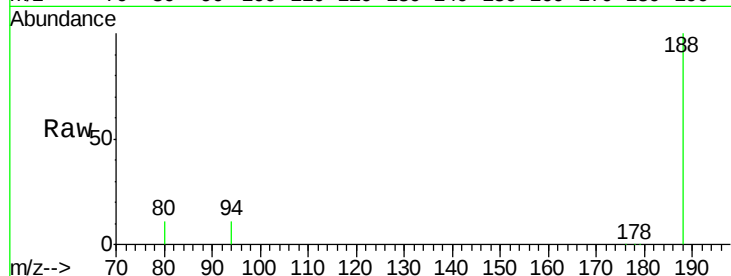

#31
Chrysene-d12
Concen: 20.00 ng
RT: 21.76 min Scan# 1064
Delta R.T. 0.00 min
Lab File: BE091986.D
Acq: 7 Jul 2016 18:23

Tgt Ion:240 Resp: 1127749
Ion Ratio Lower Upper
240 100
120 3.5 1.2 1.8#
236 31.3 19.8 29.8#

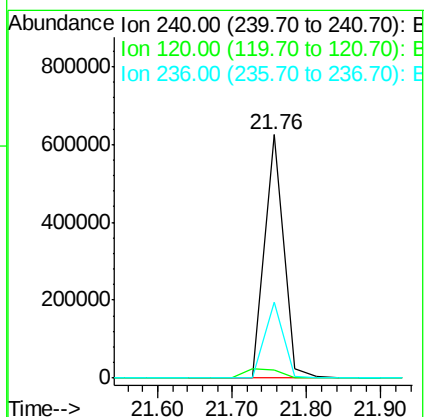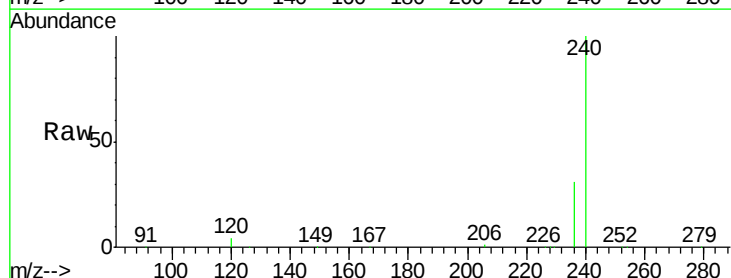

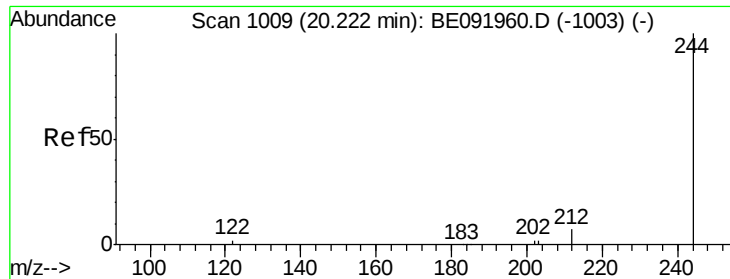

#34

Terphenyl-d14

Concen: 74.26 ng

RT: 20.22 min Scan# 1009

Delta R.T. -0.00 min

Lab File: BE091986.D

Acq: 7 Jul 2016 18:23

Instrument :

BNA_E

ClientSampleId :

FB-06202016


Tot Ion:244 Resp: 2469356

Ion Ratio Lower Upper

244 100

212 10.0 6.5 9.7#




122 1.3 2.9 4.3#

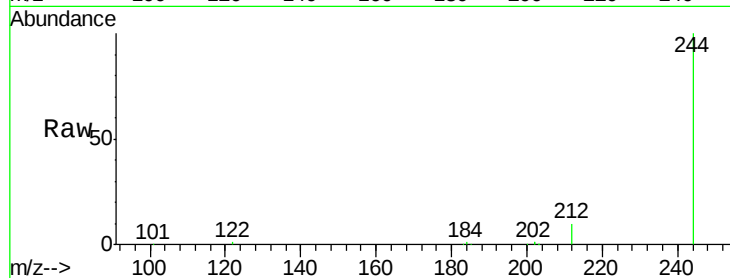

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

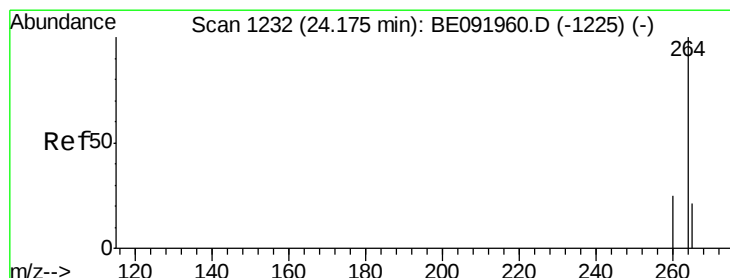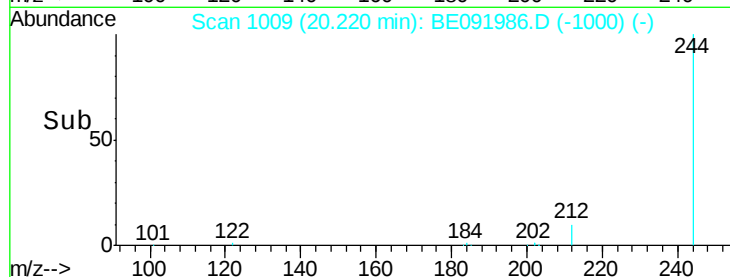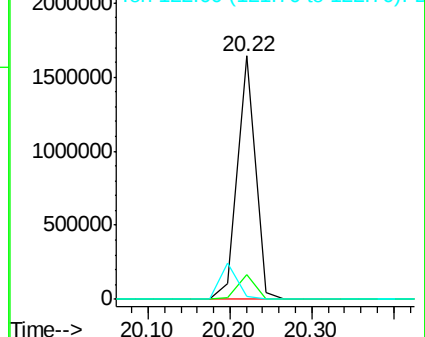

#40

Perylene-d12

Concen: 20.00 ng

RT: 24.17 min Scan# 1232

Delta R.T. 0.00 min

Lab File: BE091986.D

Acq: 7 Jul 2016 18:23


Tgt Ion:264 Resp: 1034865

Ion Ratio Lower Upper

264 100

260 26.9 20.3 30.5

265 20.9 17.6 26.4

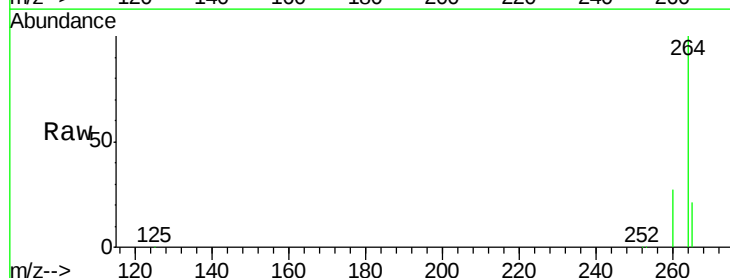

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

