


Data Path : Z:\HPCHEM1\BNA E\DATA\BE070716\
 Data File : BE091983.D
 Acq On : 7 Jul 2016 16:33
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE070516.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 05 16:14:58 2016

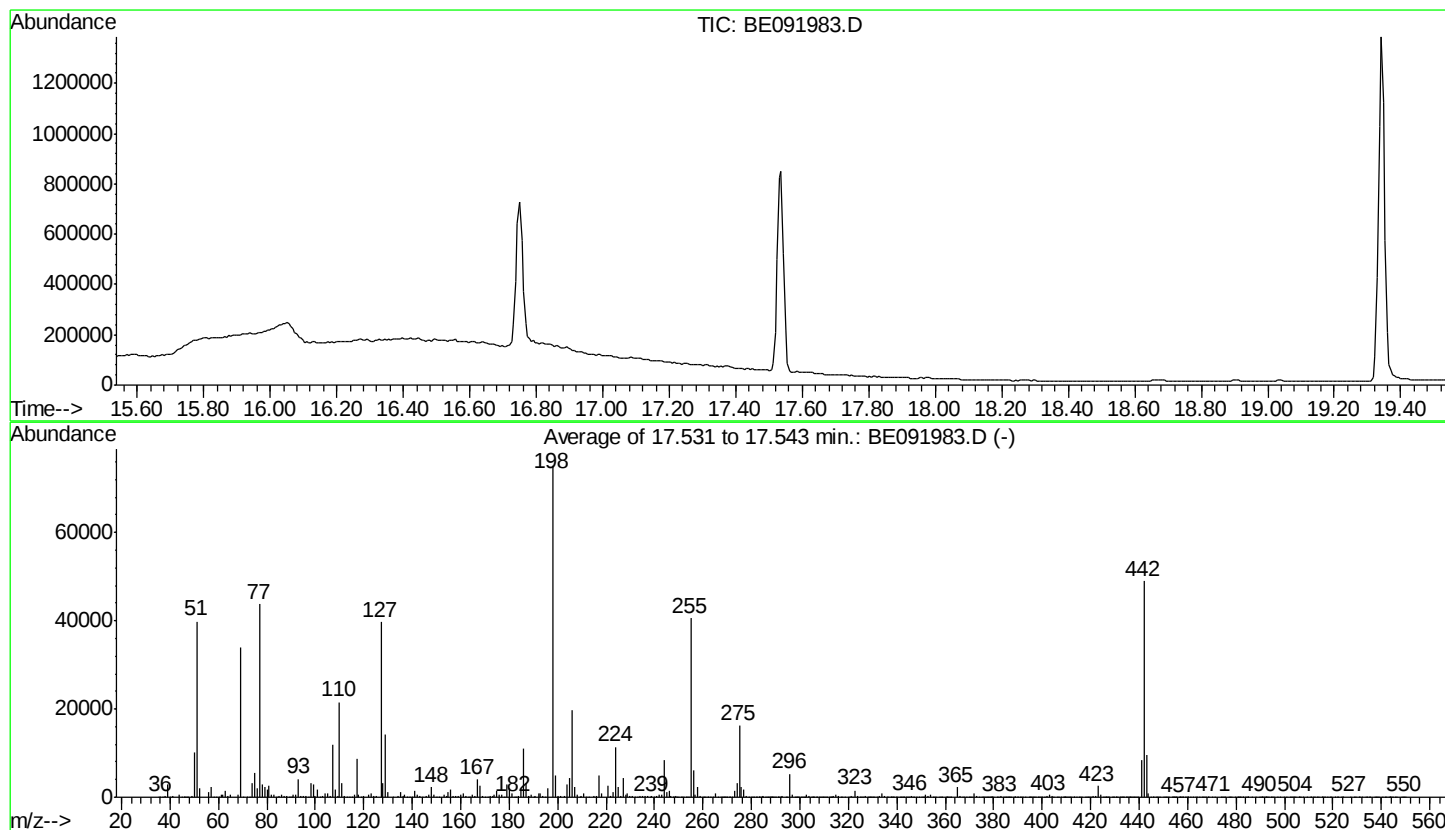

AutoFind: Scans 2543, 2544, 2545; Background Corrected with Scan 2536

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.1	39899	PASS
68	69	0.00	2	1.8	623	PASS
69	198	0.00	100	45.4	34103	PASS
70	69	0.00	2	0.3	108	PASS
127	198	10	80	52.8	39719	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	75171	PASS
199	198	5	9	6.8	5087	PASS
275	198	10	60	21.6	16245	PASS
365	198	1	100	2.9	2207	PASS
441	442	0.01	24	17.4	8515	PASS
442	198	50	100	65.2	48998	PASS
443	442	15	24	19.3	9474	PASS