


Data Path : Z:\HPCHEM1\BNA_E\Data\BE070717\
 Data File : BE093433.D
 Acq On : 7 Jul 2017 8:19
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE070217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 03 06:40:23 2017

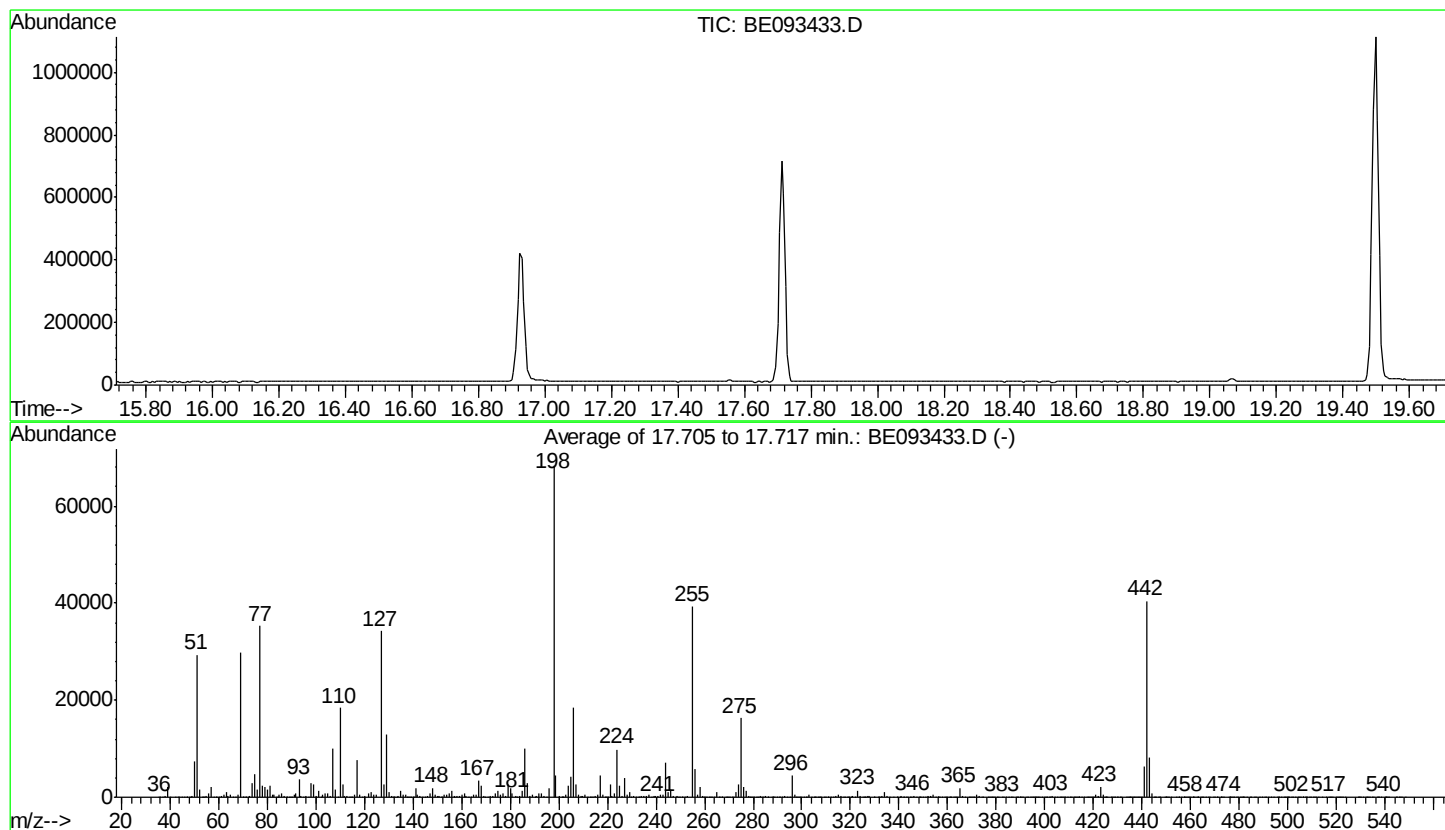

AutoFind: Scans 2573, 2574, 2575; Background Corrected with Scan 2564

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.9	29328	PASS
68	69	0.00	2	1.9	574	PASS
69	198	0.00	100	43.5	29754	PASS
70	69	0.00	2	0.5	135	PASS
127	198	10	80	50.0	34193	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	68330	PASS
199	198	5	9	6.6	4506	PASS
275	198	10	60	23.9	16348	PASS
365	198	1	100	2.8	1880	PASS
441	442	0.01	24	15.7	6340	PASS
442	198	50	100	59.1	40412	PASS
443	442	15	24	20.1	8121	PASS