


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE070815\
Data File : BE090061.D
Acq On : 8 Jul 2015 16:01
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BE062915.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jun 30 07:01:01 2015

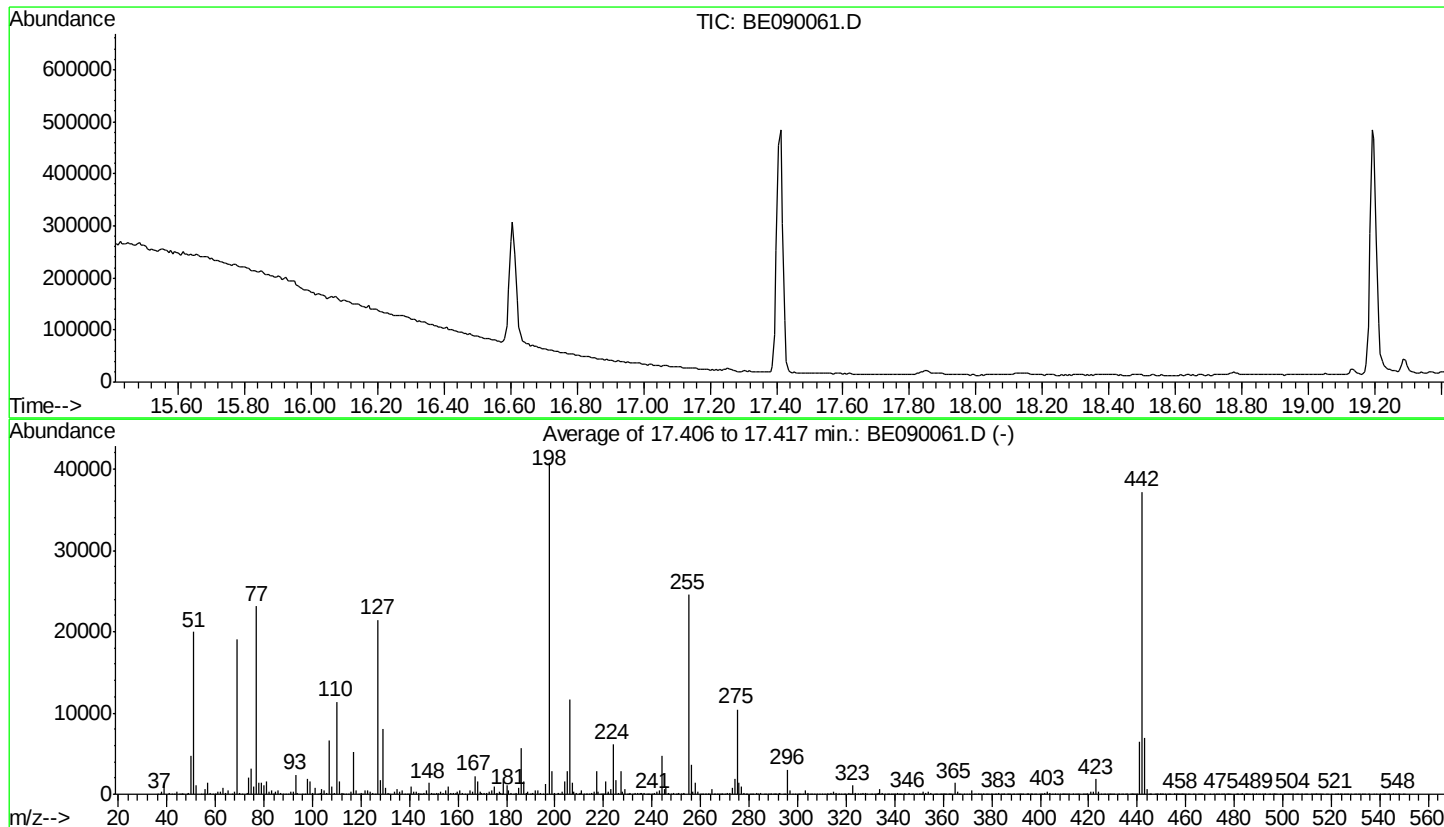

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.0	19974	PASS
68	69	0.00	2	1.9	355	PASS
69	198	0.00	100	46.7	19067	PASS
70	69	0.00	2	0.5	95	PASS
127	198	10	80	52.6	21456	PASS
197	198	0.00	2	0.1	51	PASS
198	198	100	100	100.0	40798	PASS
199	198	5	9	6.8	2767	PASS
275	198	10	60	25.7	10475	PASS
365	198	1	100	3.4	1404	PASS
441	442	0.01	24	17.3	6436	PASS
442	198	50	100	91.2	37209	PASS
443	442	15	24	18.8	7008	PASS