
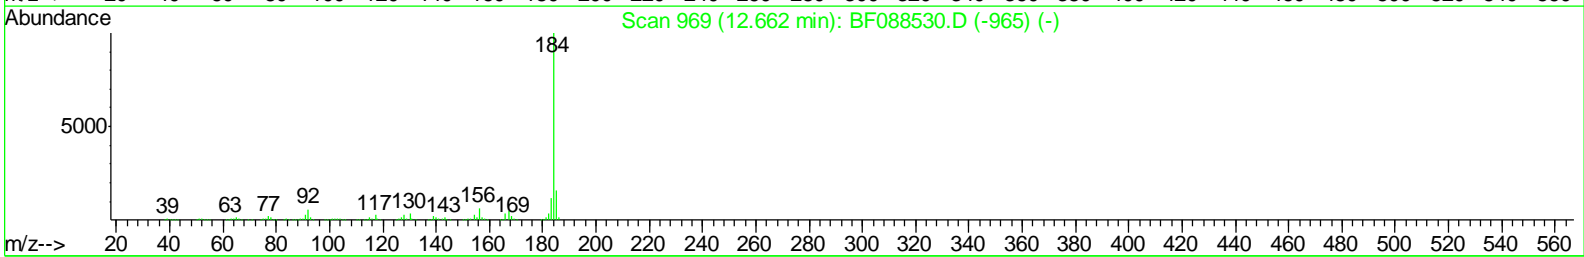
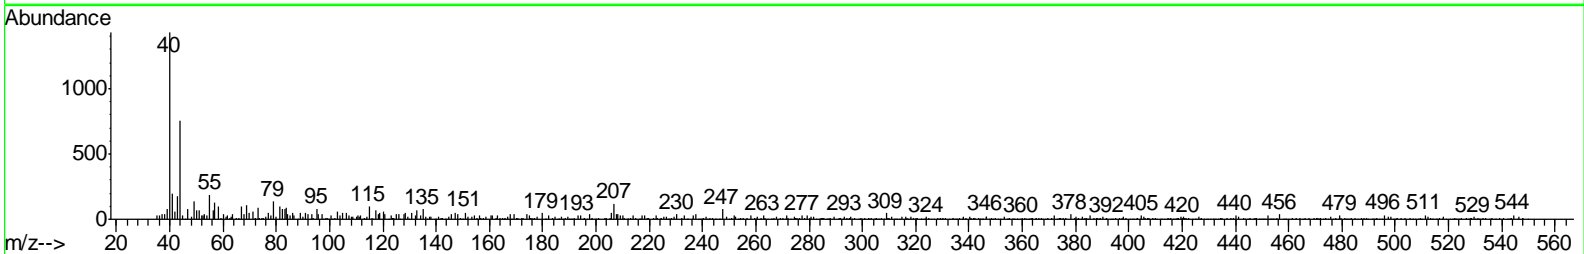


Data Path : Z:\HPCHEM1\BNA_E\Data\BE070916\
 Data File : BE091990.D
 Acq On : 9 Jul 2016 9:40
 Operator : UM/SJ
 Sample : DF7PP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 07:21:21 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 18:51:20 2016
 Response via : Initial Calibration

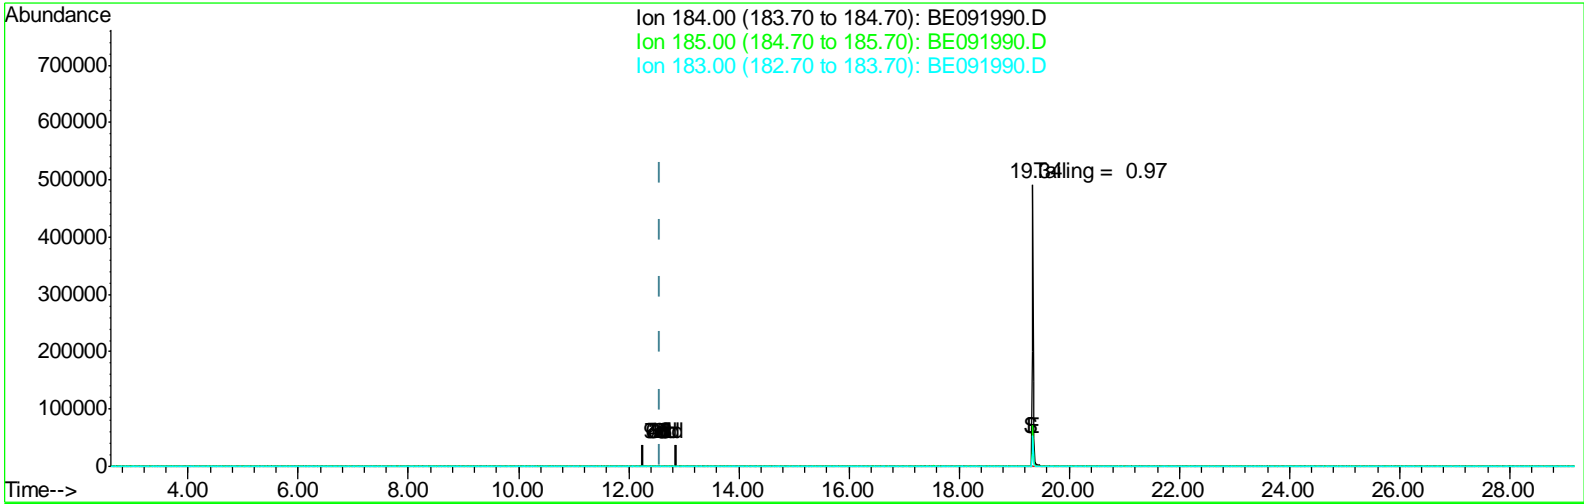

TIC: BE091990.D

(76) Benzidine




12.620min (+0.049) 34.91ng

response 30

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	7.69#
183.00	11.60	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_E\Data\BE070916\
 Data File : BE091990.D
 Acq On : 9 Jul 2016 9:40
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 11 07:21:21 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF063016.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 08 18:51:20 2016
 Response via : Initial Calibration

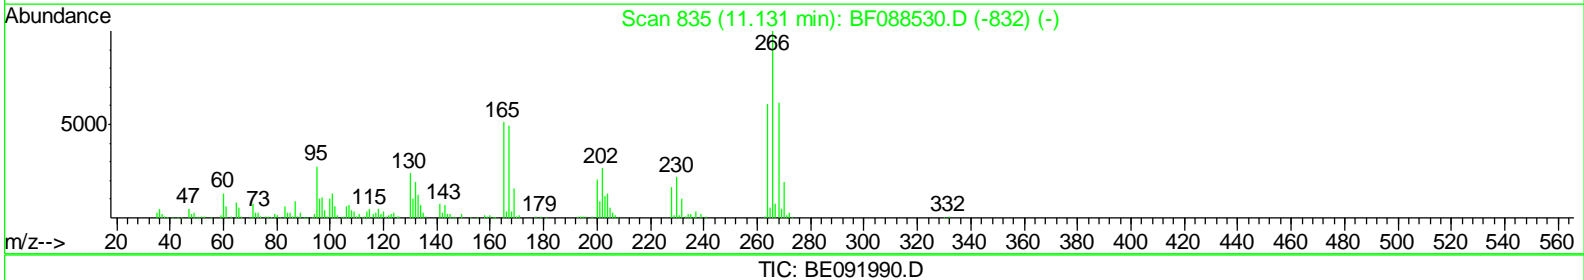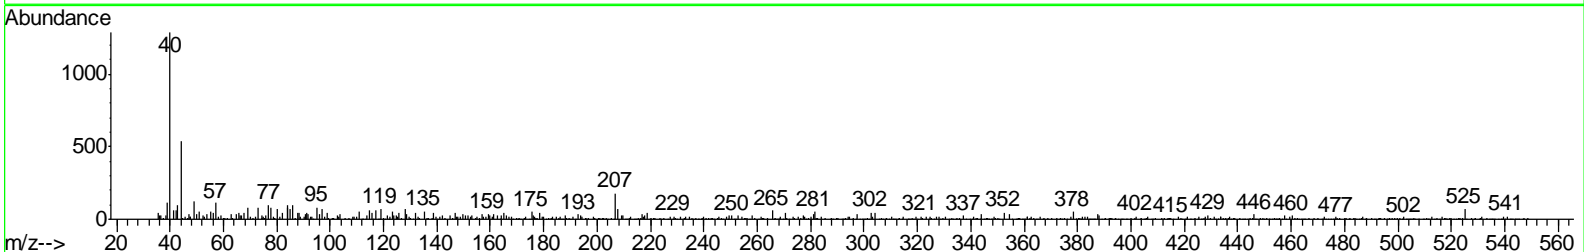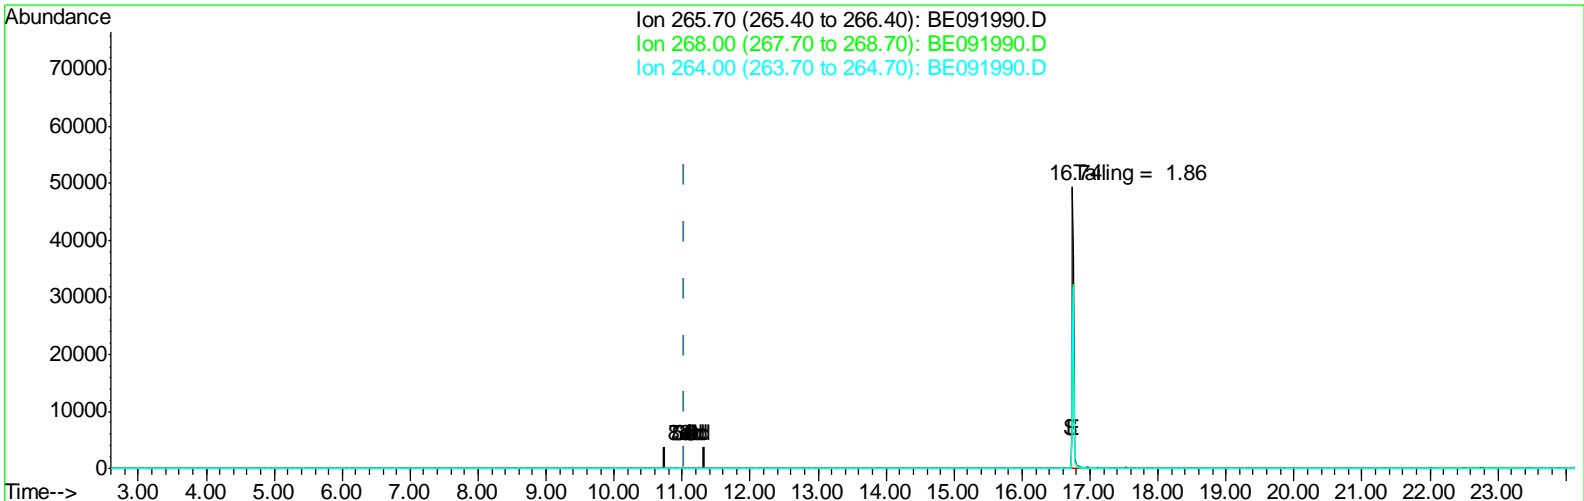

TIC: BE091990.D

(69) Pentachlorophenol (C)
 11.092min (+0.042) 331.34ng
 response 35

Ion	Exp%	Act%
265.70	100	100
268.00	66.00	36.51#
264.00	62.00	15.87#
0.00	0.00	0.00