


Data Path : V:\HPCHEM1\BNA E\DATA\BE070916\
Data File : BE091990.D
Acq On : 9 Jul 2016 9:40
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE070516.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 05 16:14:58 2016

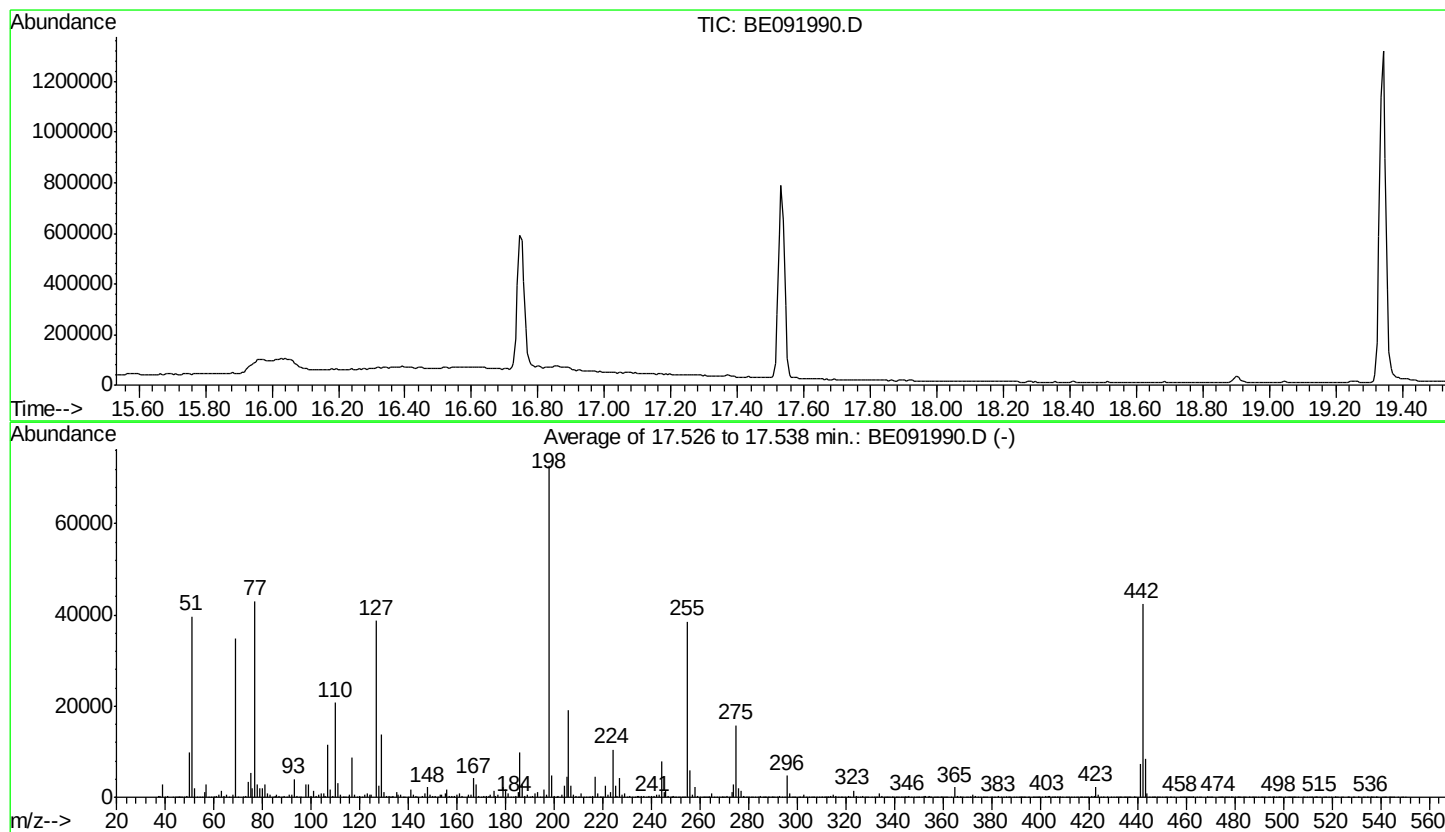

AutoFind: Scans 2542, 2543, 2544; Background Corrected with Scan 2535

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.5	39602	PASS
68	69	0.00	2	1.4	494	PASS
69	198	0.00	100	47.8	34792	PASS
70	69	0.00	2	0.4	135	PASS
127	198	10	80	53.2	38682	PASS
197	198	0.00	2	0.7	484	PASS
198	198	100	100	100.0	72715	PASS
199	198	5	9	6.7	4853	PASS
275	198	10	60	21.6	15741	PASS
365	198	1	100	3.0	2168	PASS
441	442	0.01	24	17.4	7381	PASS
442	198	50	100	58.3	42418	PASS
443	442	15	24	20.1	8525	PASS