


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE071015\
 Data File : BE090080.D
 Acq On : 10 Jul 2015 10:41
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE062915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 30 07:01:01 2015

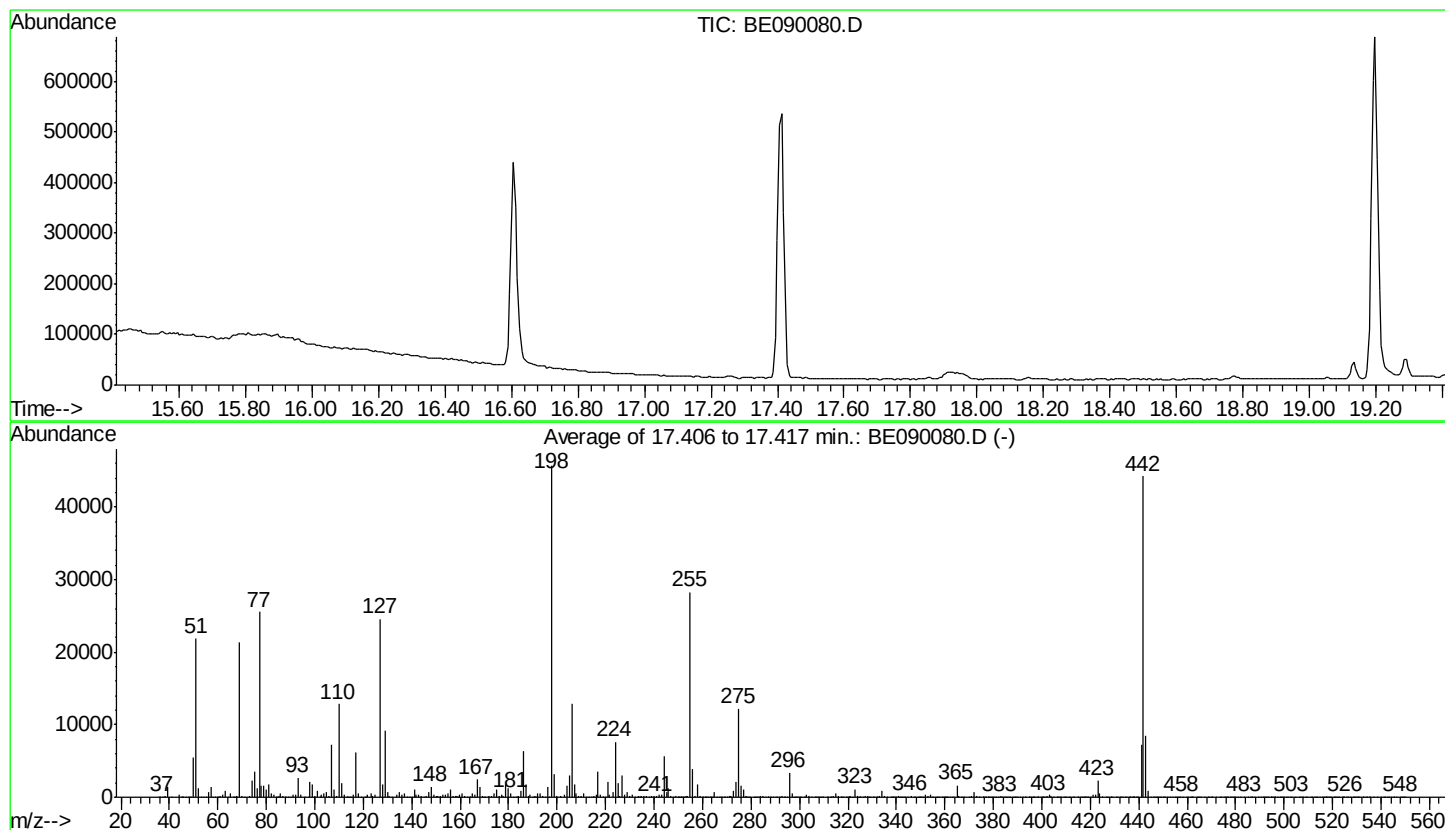

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.9	21878	PASS
68	69	0.00	2	0.9	192	PASS
69	198	0.00	100	46.8	21395	PASS
70	69	0.00	2	0.5	100	PASS
127	198	10	80	53.7	24565	PASS
197	198	0.00	2	0.1	68	PASS
198	198	100	100	100.0	45714	PASS
199	198	5	9	7.1	3238	PASS
275	198	10	60	26.7	12220	PASS
365	198	1	100	3.6	1632	PASS
441	442	0.01	24	16.5	7290	PASS
442	198	50	100	96.9	44290	PASS
443	442	15	24	19.0	8427	PASS