
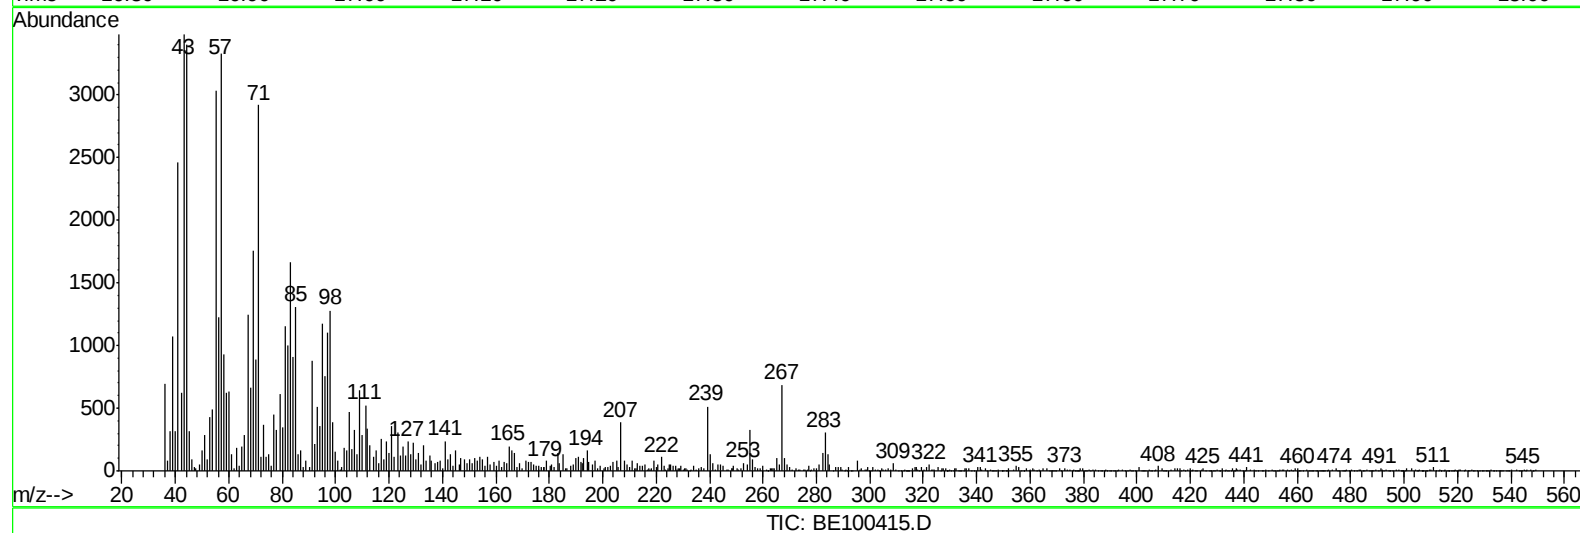


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE071219\
 Data File : BE100415.D
 Acq On : 12 Jul 2019 11:09
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 01:59:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 21 01:27:44 2013
 Response via : Initial Calibration

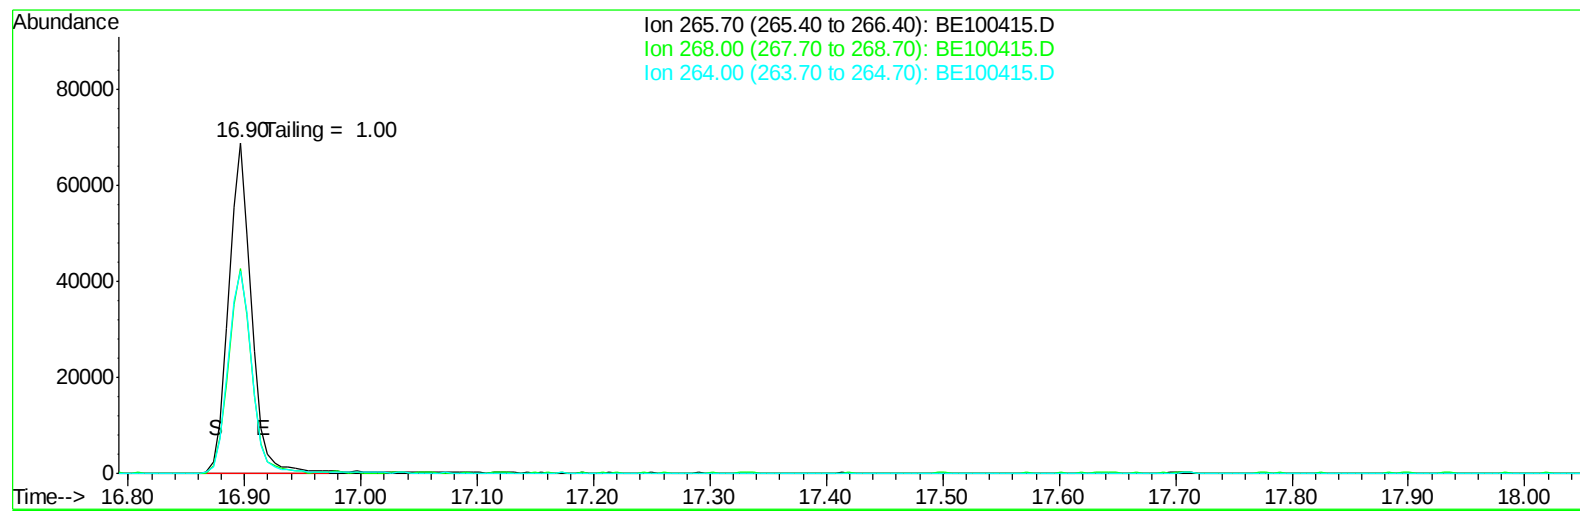

(69) Pentachlorophenol (C)



12.079min (-0.009) 189.60ng

response 41

Ion	Exp%	Act%
265.70	100	100
268.00	63.30	185.71#
264.00	65.00	67.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE071219\
 Data File : BE100415.D
 Acq On : 12 Jul 2019 11:09
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 01:59:46 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-BE111513.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 21 01:27:44 2013
 Response via : Initial Calibration

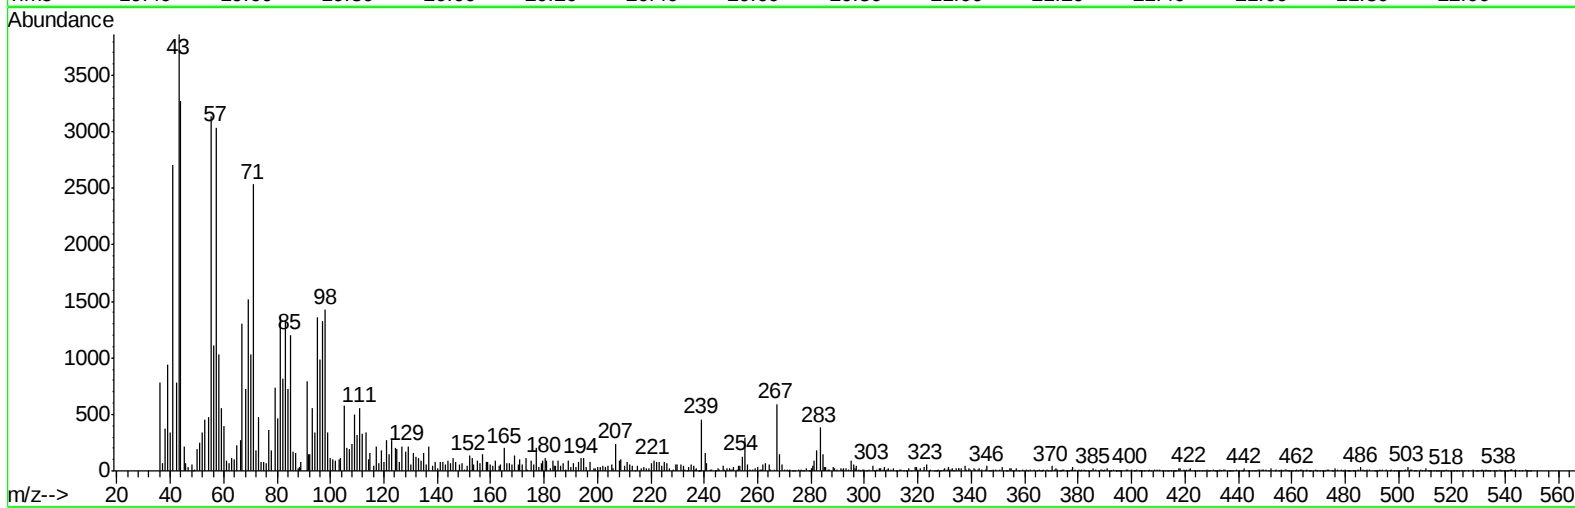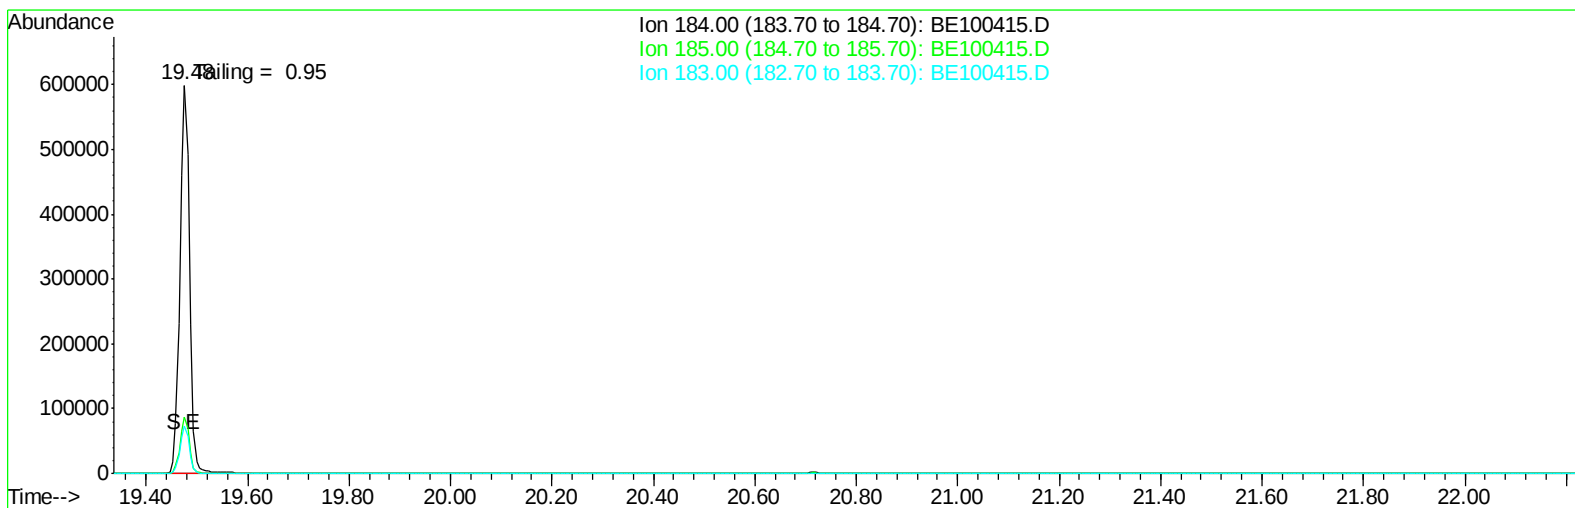

TIC: BE100415.D

(76) Benzidine

14.564min (-0.026) 129.49ng

response 105

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	97.78#
183.00	12.20	156.67#
0.00	0.00	0.00