


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE071219\
 Data File : BE100415.D
 Acq On : 12 Jul 2019 11:09
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE071219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 12 17:09:02 2019

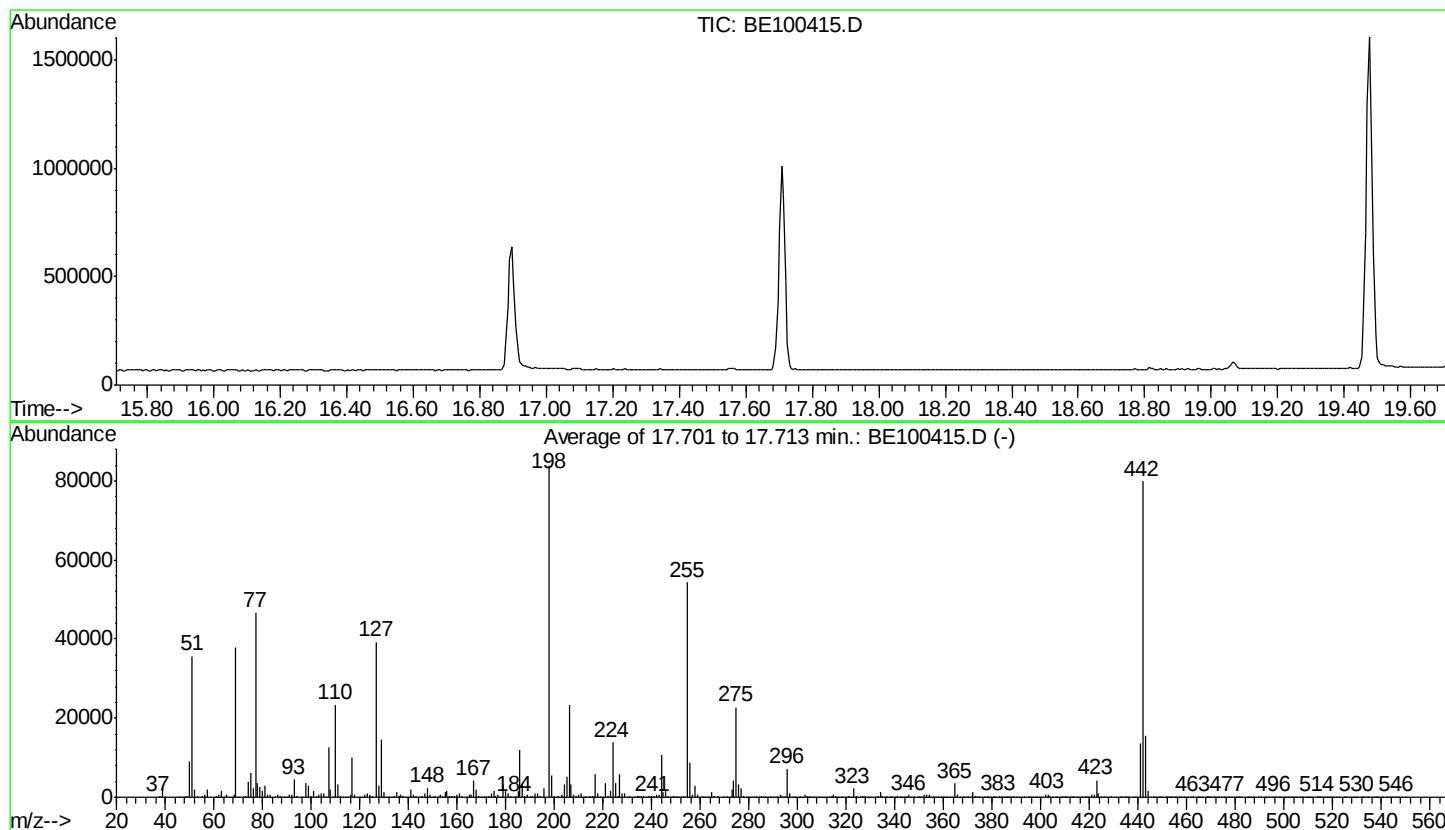

AutoFind: Scans 2572, 2573, 2574; Background Corrected with Scan 2563

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.6	35739	PASS
68	69	0.00	2	1.9	727	PASS
69	198	0.00	100	45.2	37930	PASS
70	69	0.00	2	0.2	75	PASS
127	198	10	80	46.8	39210	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83870	PASS
199	198	5	9	6.6	5536	PASS
275	198	10	60	27.1	22707	PASS
365	198	1	100	4.2	3518	PASS
441	198	0.01	100	16.4	13769	PASS
442	198	50	100	95.2	79834	PASS
443	442	15	24	19.5	15563	PASS