
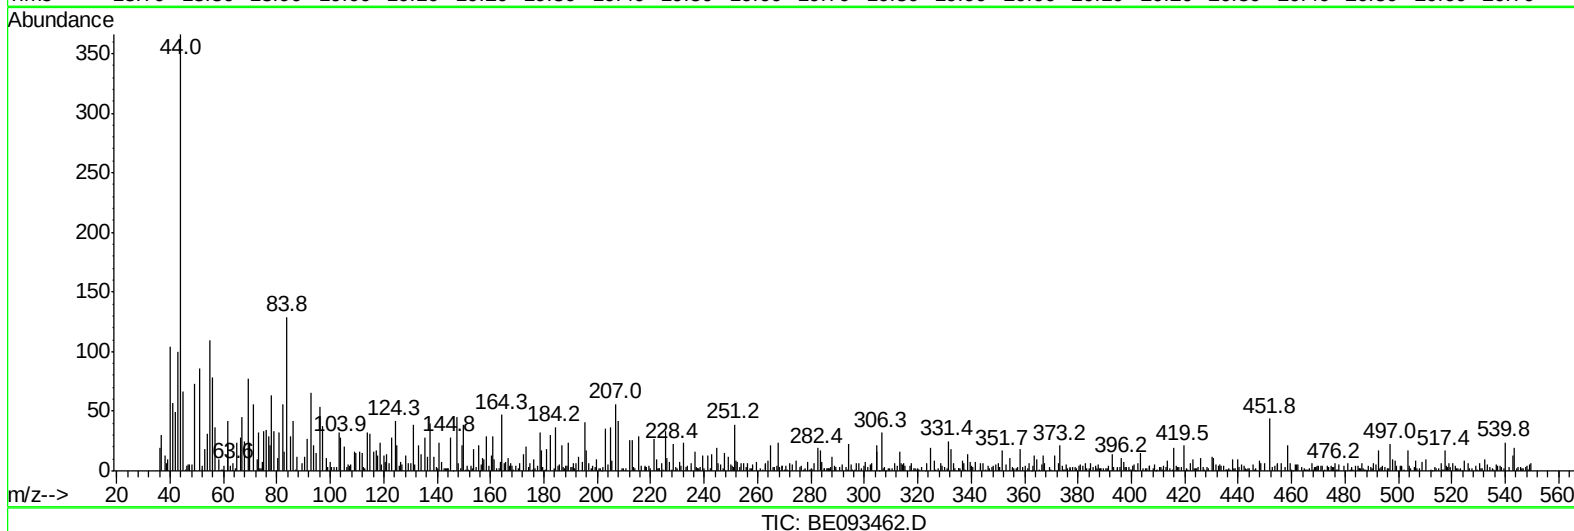


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE071417\
Data File : BE093462.D
Acq On : 14 Jul 2017 9:11
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 17 02:57:46 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 13 14:49:34 2017
Response via : Initial Calibration

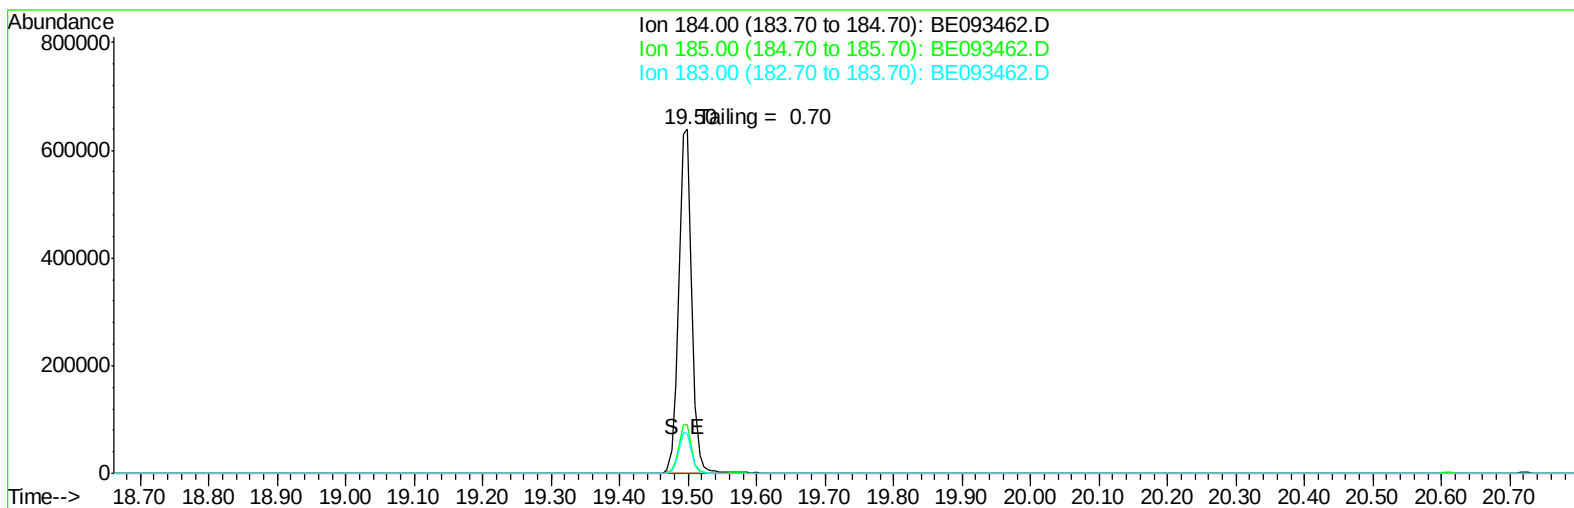

(76) Benzidine



12.525min (+0.050) 43.61ng

response 20

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	10.81#
183.00	12.20	5.41#
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA E\DATA\BE071417\
Data File : BE093462.D
Acq On : 14 Jul 2017 9:11
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 17 02:57:46 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF071317.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 13 14:49:34 2017
Response via : Initial Calibration

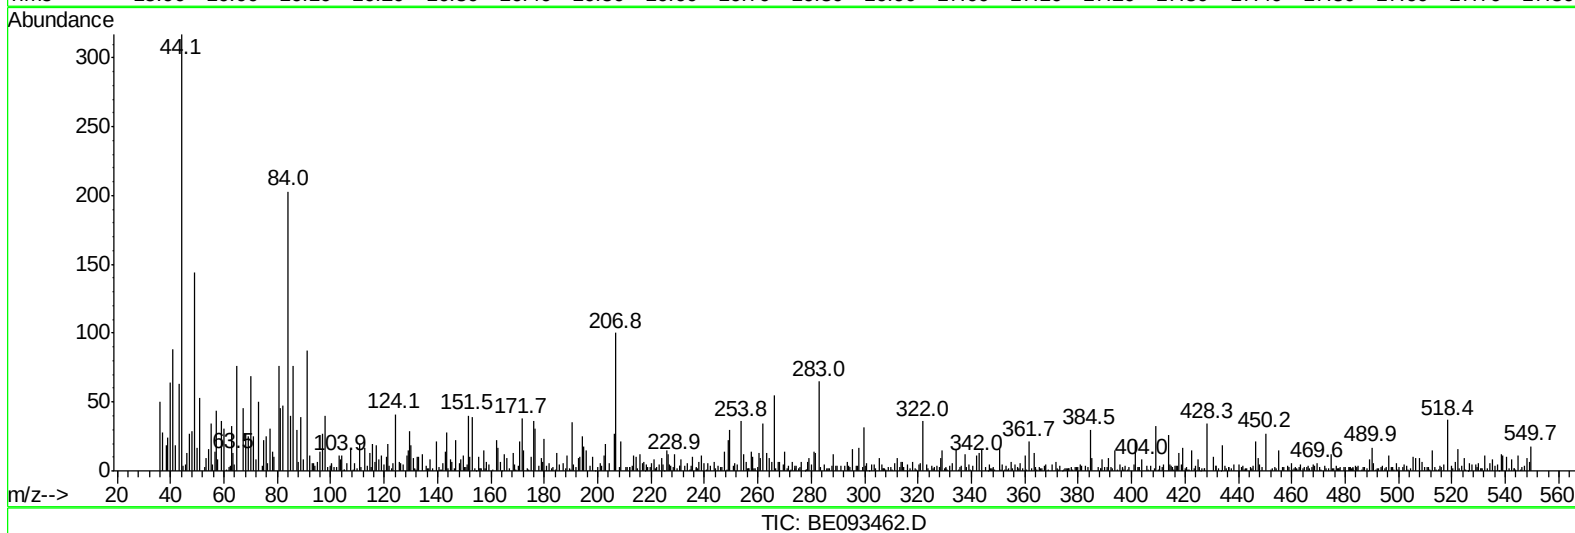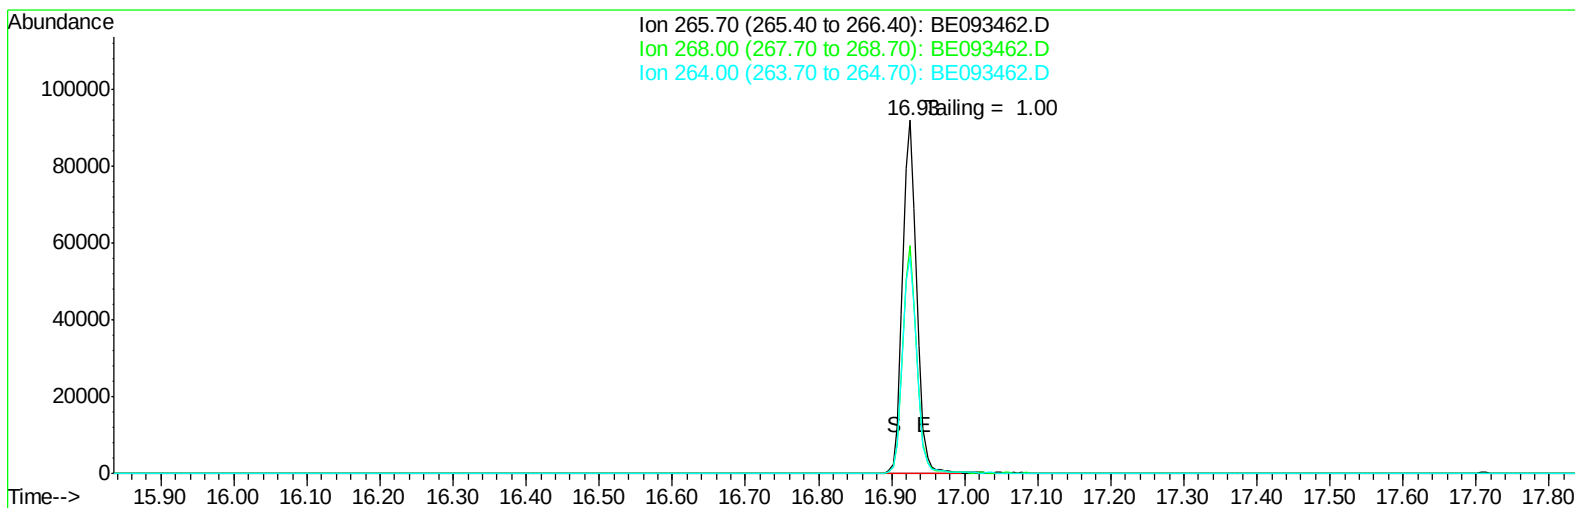

(69) Pentachlorophenol (C)

10.997min (+0.040) 307.19ng

response 27

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	25.45#
264.00	64.60	16.36#
0.00	0.00	0.00