


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA E\Data\BE071417\
 Data File : BE093462.D
 Acq On : 14 Jul 2017 9:11
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE070217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 03 06:40:23 2017

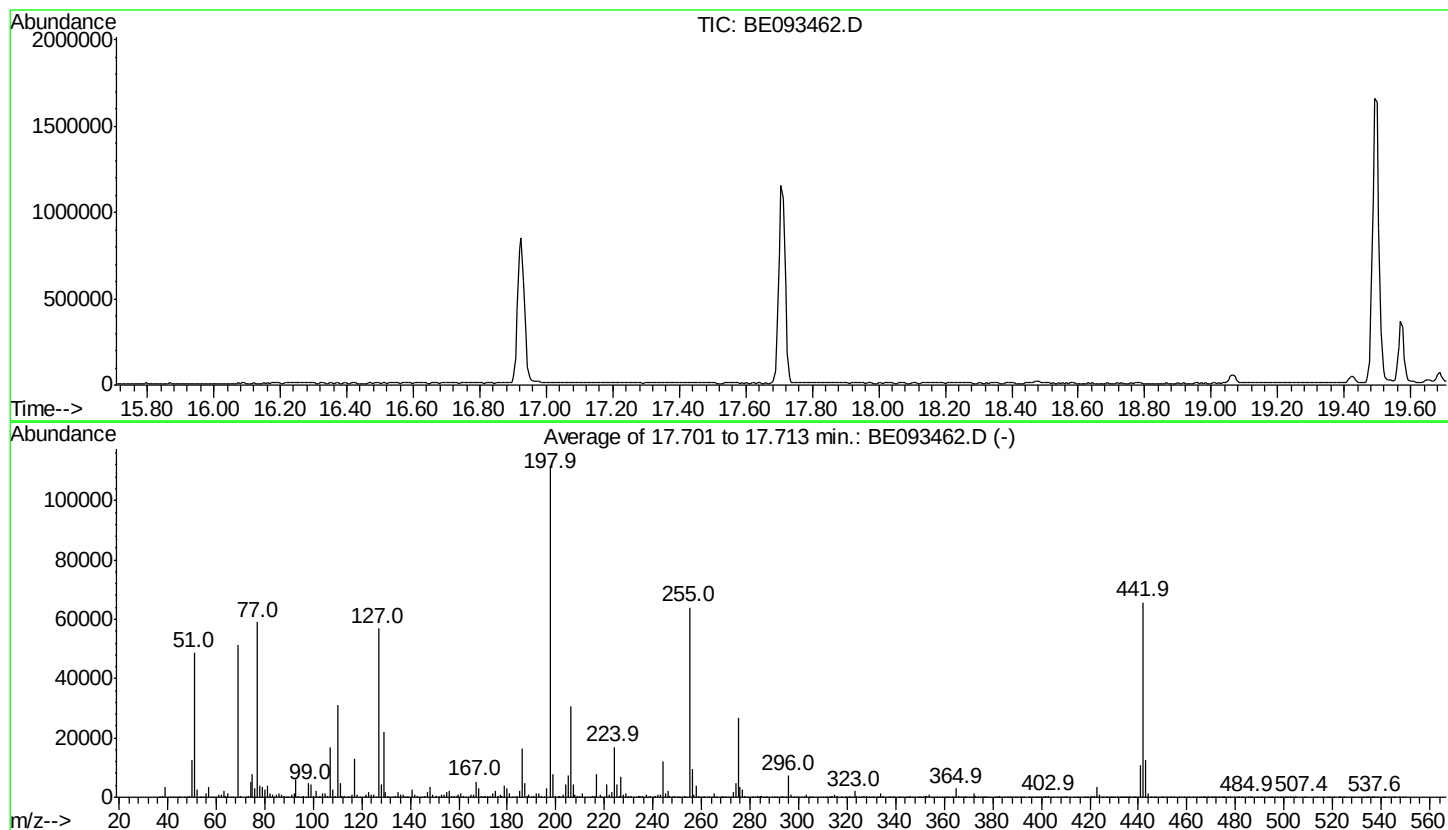

AutoFind: Scans 2572, 2573, 2574; Background Corrected with Scan 2564

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.6	48736	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	45.8	51141	PASS
70	69	0.00	2	0.6	294	PASS
127	198	10	80	50.9	56902	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	111760	PASS
199	198	5	9	6.9	7690	PASS
275	198	10	60	24.1	26955	PASS
365	198	1	100	2.5	2841	PASS
441	442	0.01	24	16.2	10616	PASS
442	198	50	100	58.7	65586	PASS
443	442	15	24	19.1	12552	PASS