

Data Path : Z:\HPCHEM1\BNA\_E\DATA\BE071615\  
 Data File : BE090145.D  
 Acq On : 17 Jul 2015 7:42  
 Operator : TP/IZ  
 Sample : G3009-02  
 Misc :  
 ALS Vial : 20 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 FB-01-071515

Quant Time: Jul 17 13:47:27 2015  
 Quant Method : Z:\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE071615.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jul 17 12:59:41 2015  
 Response via : Initial Calibration


| Internal Standards             | R.T.  | QIon | Response | Conc | Units | Dev(Min)     |
|--------------------------------|-------|------|----------|------|-------|--------------|
| 1) 1,4-Dichlorobenzene-d4      | 7.61  | 152  | 13297    | 5.00 | ng    | 0.00         |
| 6) Naphthalene-d8              | 10.37 | 136  | 64687    | 5.00 | ng    | 0.00         |
| 12) Acenaphthene-d10           | 14.22 | 164  | 37054    | 5.00 | ng    | 0.00         |
| 18) Phenanthrene-d10           | 16.96 | 188  | 83543    | 5.00 | ng    | 0.00         |
| 25) Chrysene-d12               | 21.12 | 240  | 87268    | 5.00 | ng    | 0.00         |
| 32) Perylene-d12               | 23.44 | 264  | 78321    | 5.00 | ng    | 0.00         |
| System Monitoring Compounds    |       |      |          |      |       |              |
| 4) 2-Fluorophenol              | 5.24  | 112  | 6976     | 2.45 | ng    | 0.00         |
| 5) Phenol-d6                   | 6.80  | 99   | 6290     | 1.56 | ng    | 0.00         |
| 7) Nitrobenzene-d5             | 8.75  | 82   | 14293    | 2.98 | ng    | 0.00         |
| 13) 2,4,6-Tribromophenol       | 15.73 | 330  | 6785     | 6.36 | ng    | 0.00         |
| 14) 2-Fluorobiphenyl           | 12.85 | 172  | 32760    | 2.87 | ng    | 0.00         |
| 27) Terphenyl-d14              | 19.58 | 244  | 59427    | 4.06 | ng    | 0.00         |
| Target Compounds               |       |      |          |      |       |              |
| 30) Bis(2-ethylhexyl)phthalate | 21.05 | 149  | 1122     | 0.40 | ng    | Qvalue<br>98 |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA\_E\DATA\BE071615\  
Data File : BE090145.D  
Acq On : 17 Jul 2015 7:42  
Operator : TP/IZ  
Sample : G3009-02  
Misc :  
ALS Vial : 20 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
FB-01-071515

Quant Time: Jul 17 13:47:27 2015  
Quant Method : Z:\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE071615.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jul 17 12:59:41 2015  
Response via : Initial Calibration

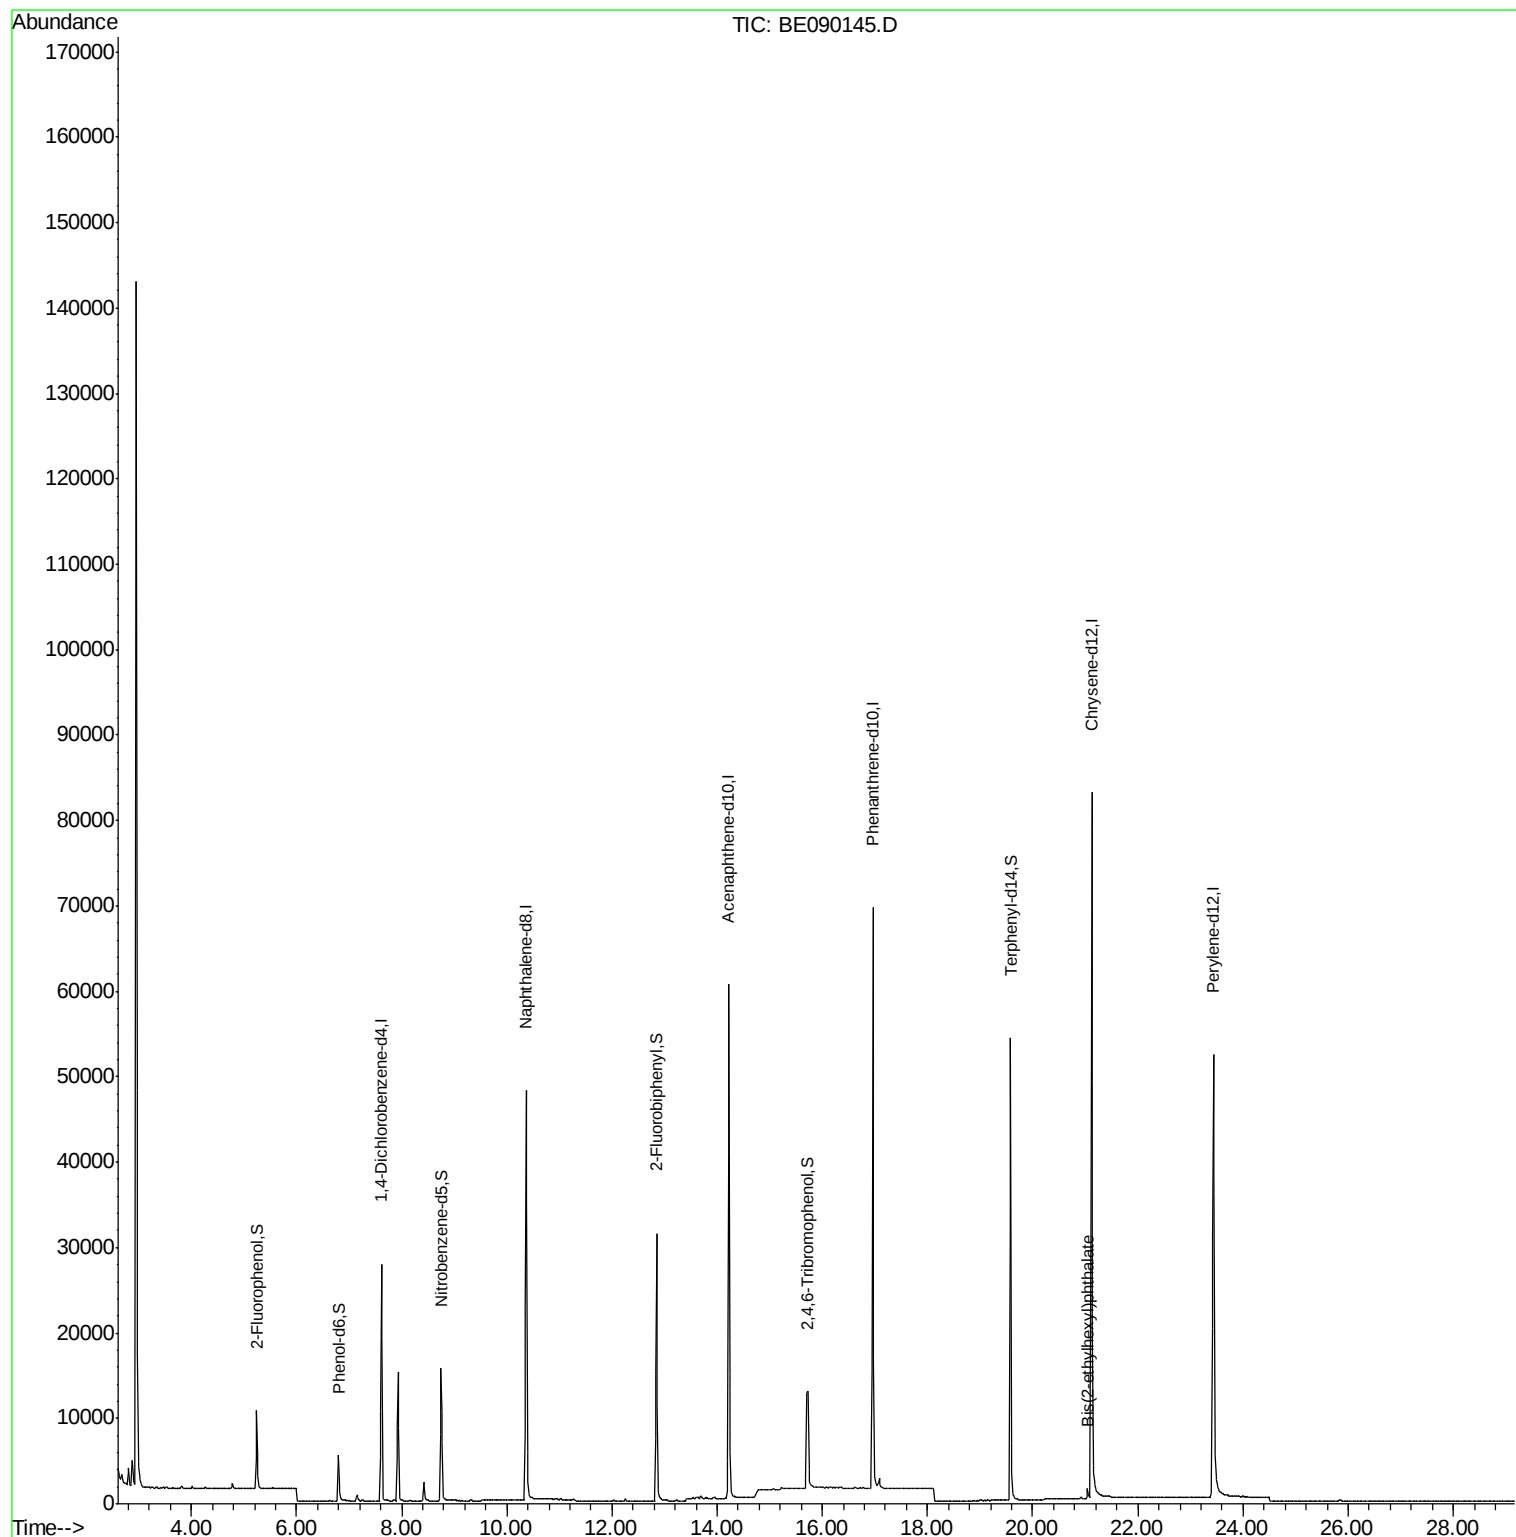




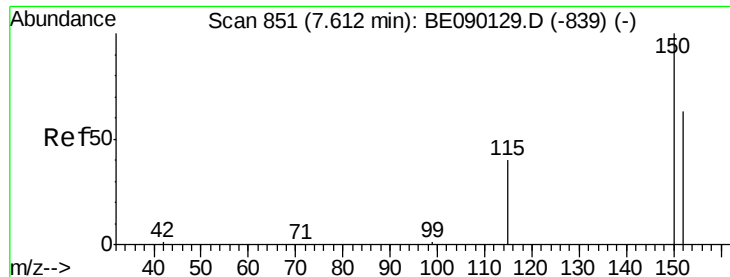


#1

1,4-Dichlorobenzene-d4  
Concen: 5.00 ng  
RT: 7.61 min Scan# 851  
Delta R.T. 0.00 min  
Lab File: BE090145.D  
Acq: 17 Jul 2015 7:42

Instrument :  
BNA\_E  
ClientSampleId :  
FB-01-071515




Tgt Ion:152 Resp: 13297  
Ion Ratio Lower Upper  
152 100  
150 158.1 127.3 190.9  
115 64.9 51.0 76.4

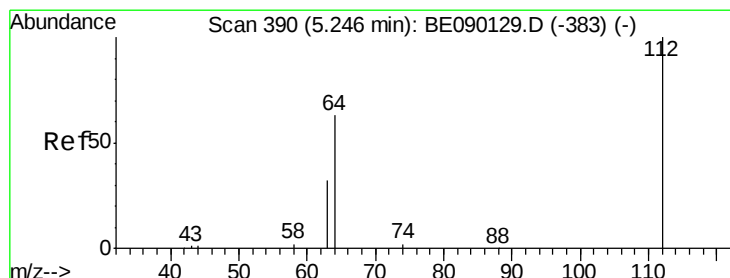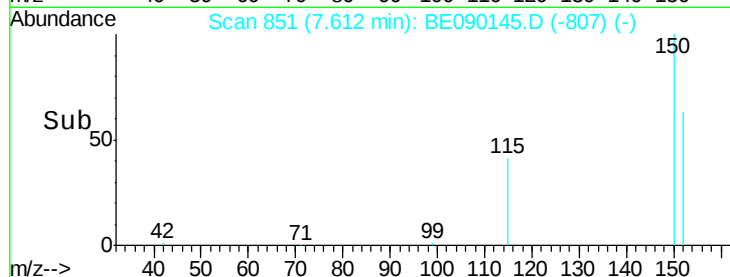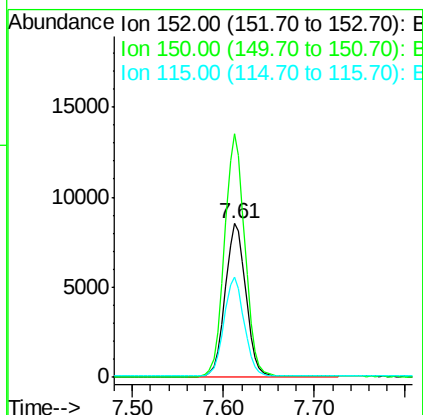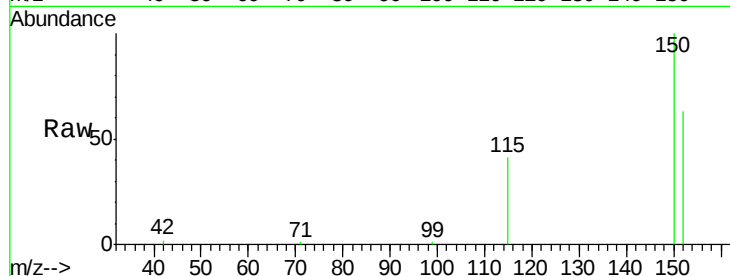


#4

2-Fluorophenol  
Concen: 2.45 ng  
RT: 5.24 min Scan# 390  
Delta R.T. -0.00 min  
Lab File: BE090145.D  
Acq: 17 Jul 2015 7:42

Tgt Ion:112 Resp: 6976  
Ion Ratio Lower Upper  
112 100  
64 68.2 55.4 83.2  
63 35.6 29.3 43.9

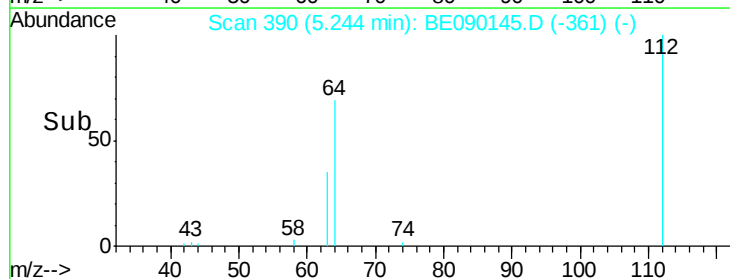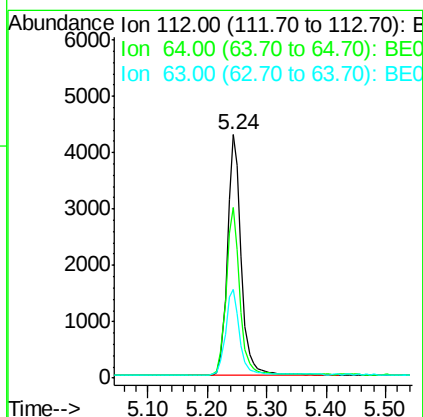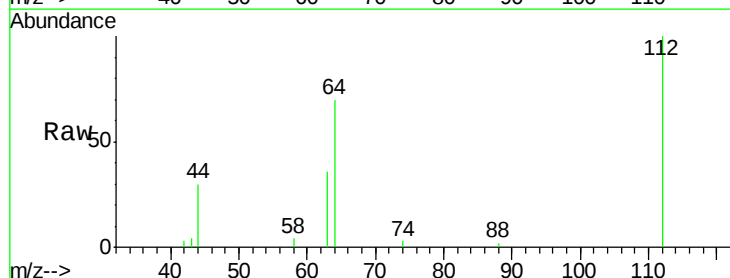

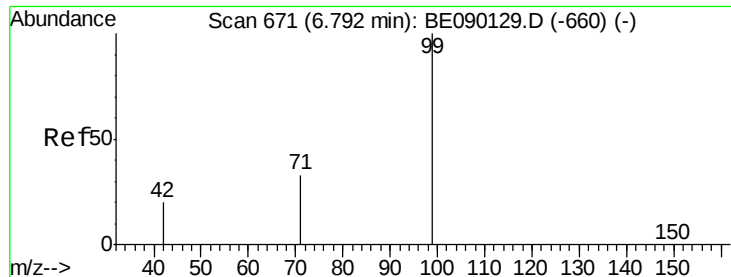

#5

Phenol-d6

Concen: 1.56 ng

RT: 6.80 min Scan# 672

Delta R.T. 0.00 min

Lab File: BE090145.D

Acq: 17 Jul 2015 7:42

Instrument :

BNA\_E

ClientSampleId :

FB-01-071515


Tgt Ion: 99 Resp: 6290

Ion Ratio Lower Upper




99 100

42 19.2 16.8 25.2

71 33.1 26.6 39.8

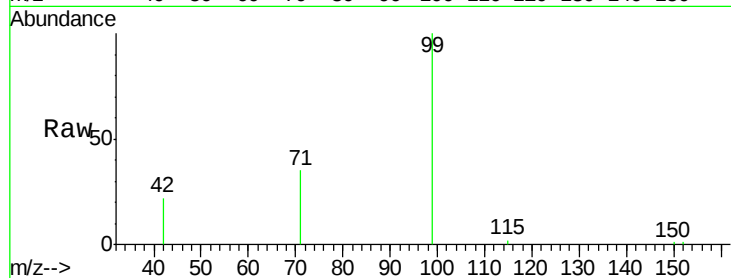

Abundance Ion 99.00 (98.70 to 99.70): BE0  
Ion 42.00 (41.70 to 42.70): BE0  
Ion 71.00 (70.70 to 71.70): BE0

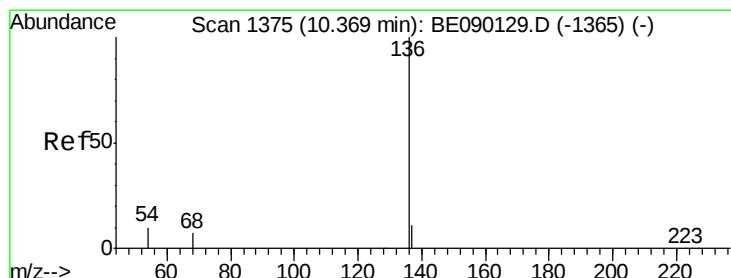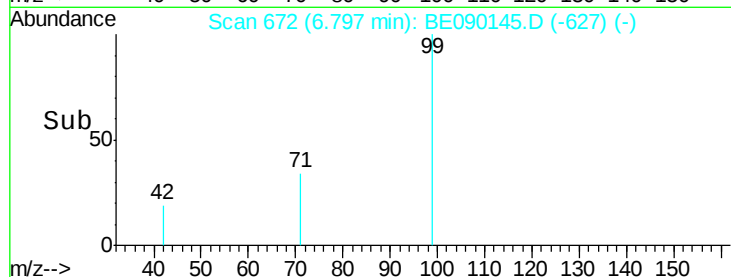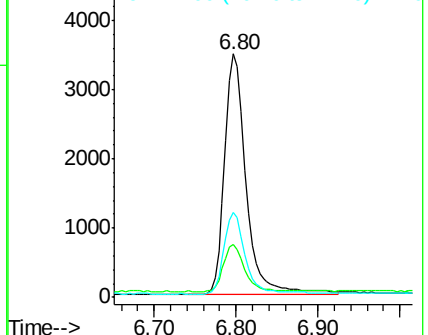

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.37 min Scan# 1375

Delta R.T. 0.00 min

Lab File: BE090145.D

Acq: 17 Jul 2015 7:42

Tgt Ion: 136 Resp: 64687


Ion Ratio Lower Upper

136 100



137 11.0 8.9 13.3


54 10.3 7.8 11.8

68 7.9 5.8 8.8

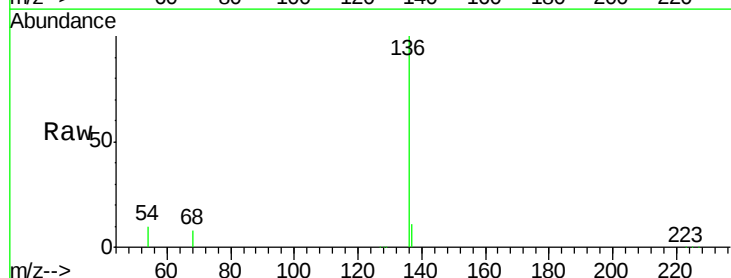

Abundance Ion 136.00 (135.70 to 136.70): E  
Ion 137.00 (136.70 to 137.70): E  
Ion 54.00 (53.70 to 54.70): BE0  
Ion 68.00 (67.70 to 68.70): BE0

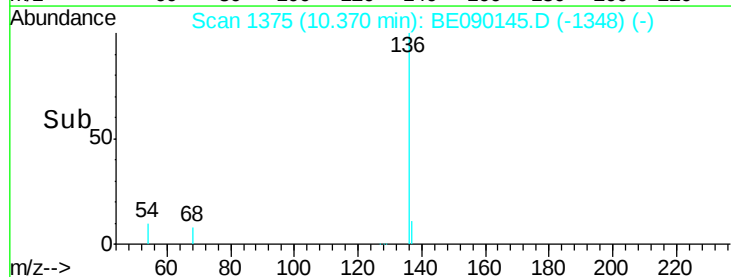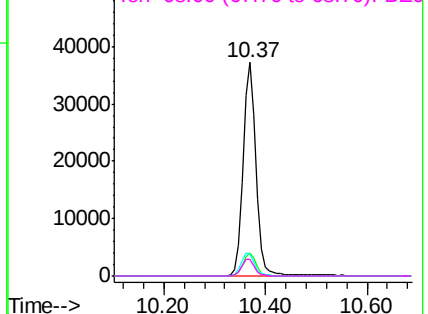

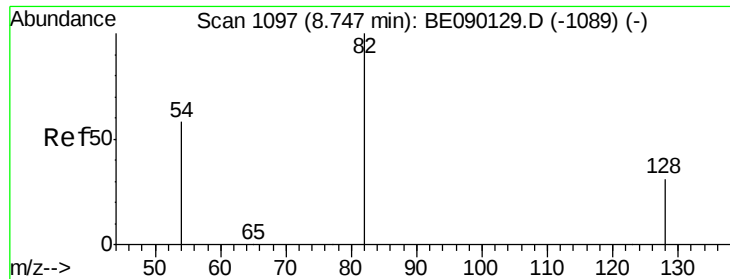

#7

Nitrobenzene-d5

Concen: 2.98 ng

RT: 8.75 min Scan# 1098

Delta R.T. 0.00 min

Lab File: BE090145.D

Acq: 17 Jul 2015 7:42

Instrument :

BNA\_E

ClientSampleId :

FB-01-071515


Tgt Ion: 82 Resp: 14293

Ion Ratio Lower Upper

82 100

128 35.4 26.2 39.2

54 54.8 47.1 70.7

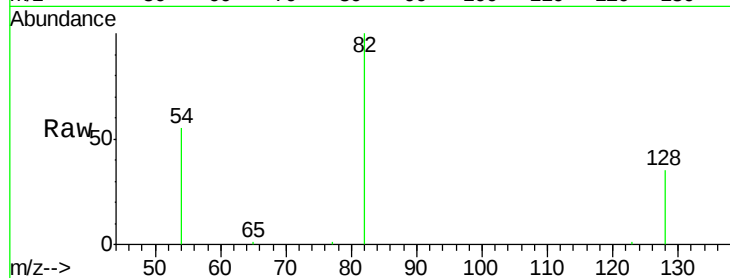


Abundance Ion 82.00 (81.70 to 82.70): BE0


Ion 128.00 (127.70 to 128.70): BE0

Ion 54.00 (53.70 to 54.70): BE0

Time-->

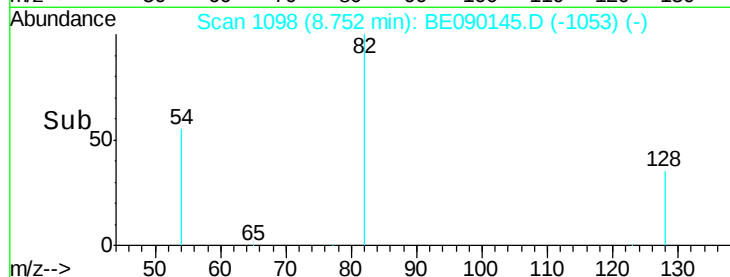

Time-->

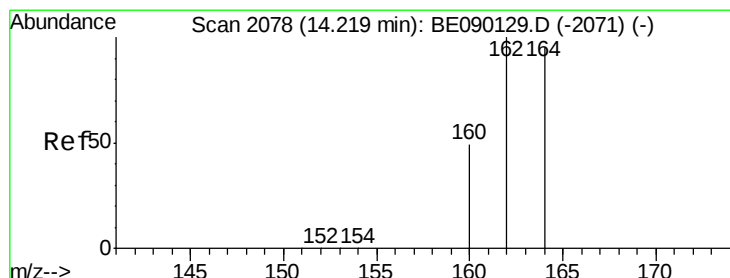

#12

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.22 min Scan# 2079

Delta R.T. 0.00 min

Lab File: BE090145.D

Acq: 17 Jul 2015 7:42


Tgt Ion: 164 Resp: 37054

Ion Ratio Lower Upper

164 100

162 105.4 84.0 126.0

160 49.4 41.1 61.7

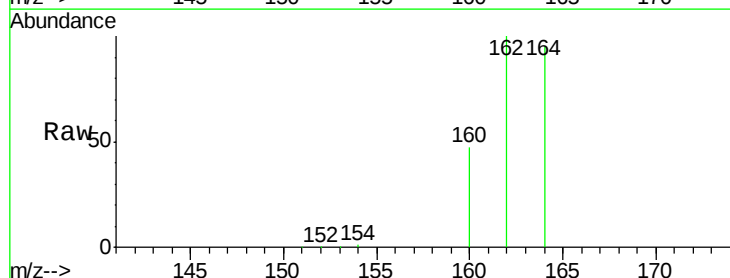


Abundance Ion 164.00 (163.70 to 164.70): E


Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

Time-->

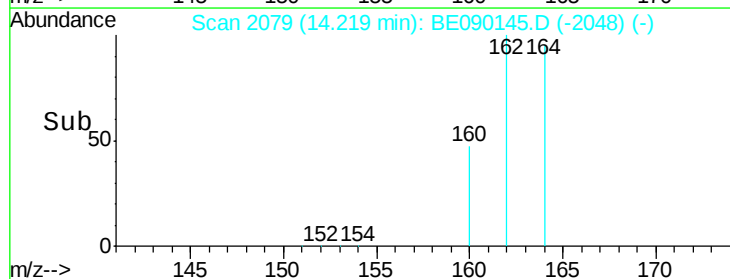


Time-->

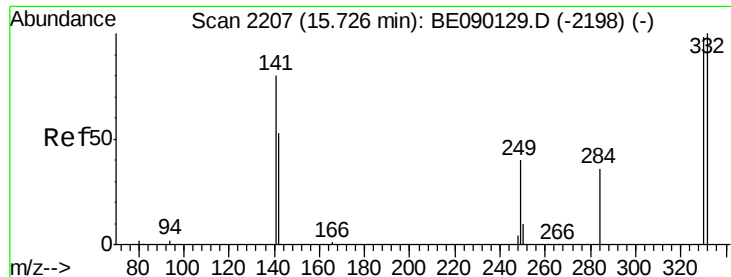




#13  
 2,4,6-Tribromophenol  
 Concen: 6.36 ng  
 RT: 15.73 min Scan# 2208  
 Delta R.T. 0.00 min  
 Lab File: BE090145.D  
 Acq: 17 Jul 2015 7:42

Instrument :  
 BNA\_E  
 ClientSampleId :  
 FB-01-071515

Tgt Ion:330 Resp: 6785  
 Ion Ratio Lower Upper  
 330 100  
 332 97.1 79.4 119.0  
 141 162.6 160.2 240.2

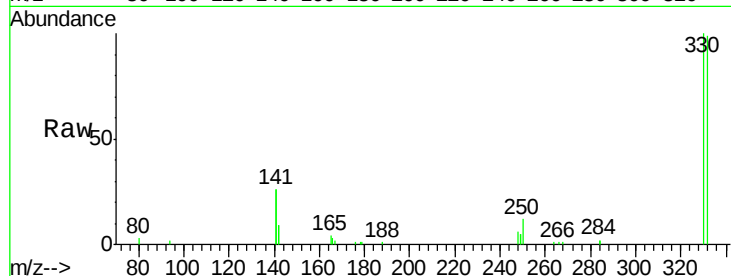


Abundance Ion 329.80 (329.50 to 330.50): E  
 Ion 331.80 (331.50 to 332.50): E  
 Ion 141.00 (140.70 to 141.70): E

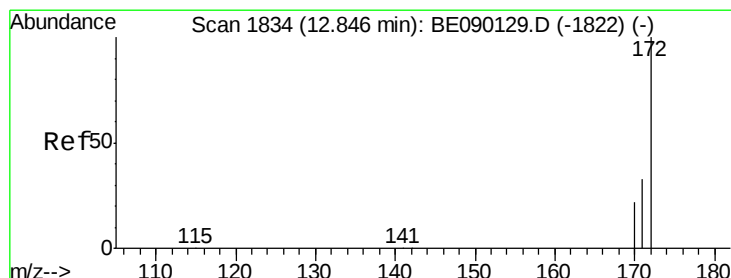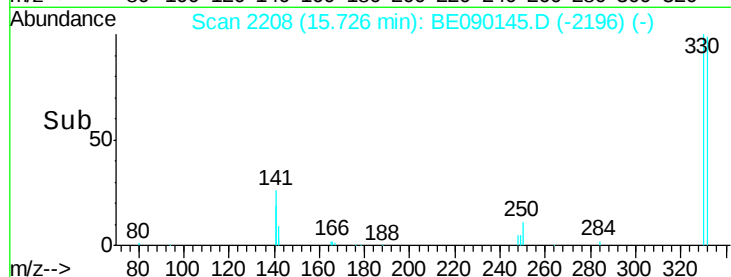
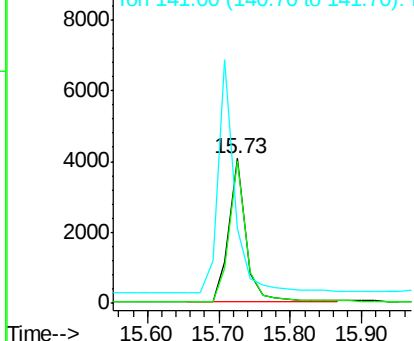



#14  
 2-Fluorobiphenyl  
 Concen: 2.87 ng  
 RT: 12.85 min Scan# 1834  
 Delta R.T. -0.00 min  
 Lab File: BE090145.D  
 Acq: 17 Jul 2015 7:42

Tgt Ion:172 Resp: 32760  
 Ion Ratio Lower Upper  
 172 100  
 171 34.6 27.1 40.7  
 170 22.9 17.9 26.9

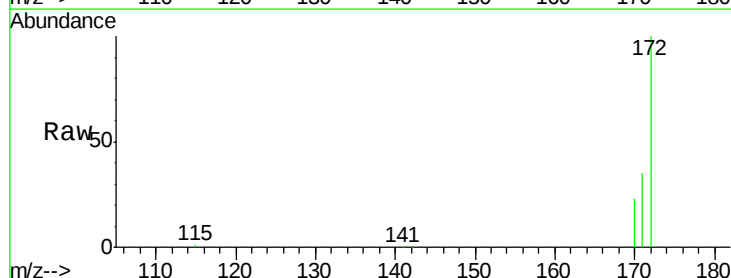

Abundance Ion 172.00 (171.70 to 172.70): E  
 Ion 171.00 (170.70 to 171.70): E  
 Ion 170.00 (169.70 to 170.70): E

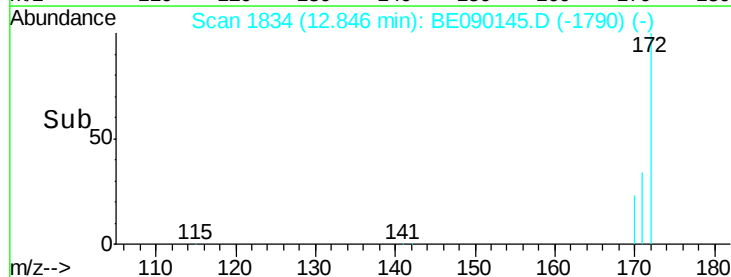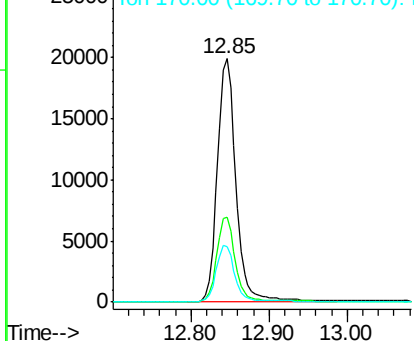

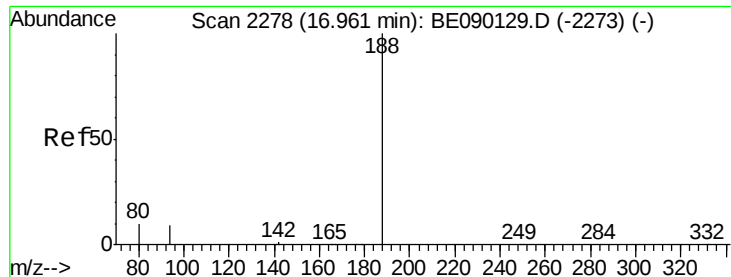

#18

Phenanthrene-d10

Concen: 5.00 ng

RT: 16.96 min Scan# 2279

Delta R.T. -0.00 min

Lab File: BE090145.D

Acq: 17 Jul 2015 7:42

Instrument :

BNA\_E

ClientSampleId :

FB-01-071515


Tgt Ion:188 Resp: 83543

Ion Ratio Lower Upper

188 100

94 9.5 7.3 10.9




80 10.4 8.0 12.0

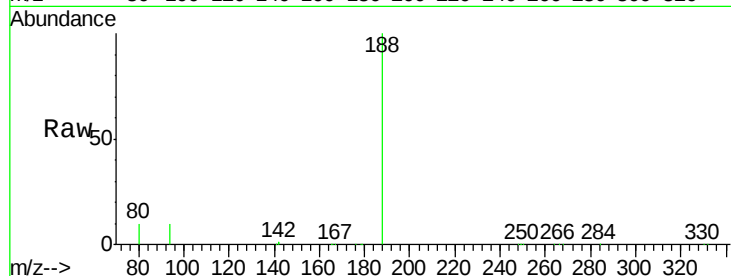

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE0

Ion 80.00 (79.70 to 80.70): BE0

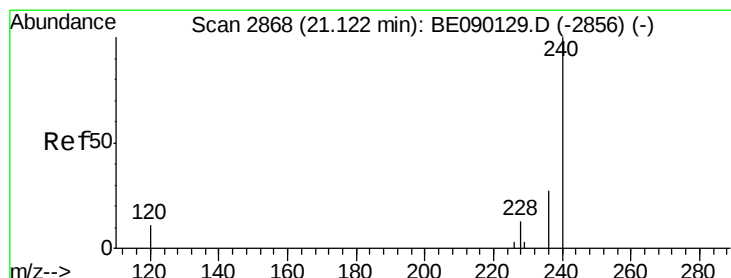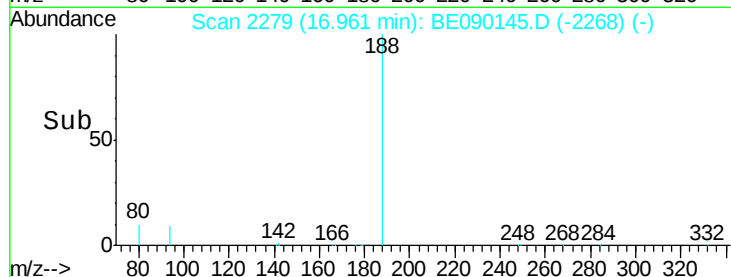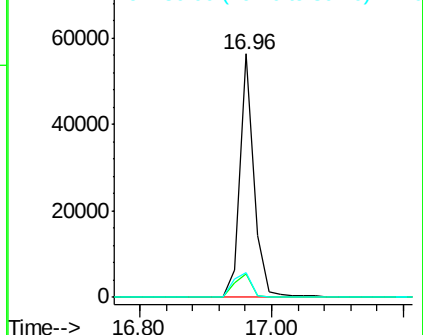

#25

Chrysene-d12

Concen: 5.00 ng

RT: 21.12 min Scan# 2869

Delta R.T. -0.00 min

Lab File: BE090145.D

Acq: 17 Jul 2015 7:42


Tgt Ion:240 Resp: 87268

Ion Ratio Lower Upper

240 100

120 9.1 8.8 13.2



236 26.0 21.4 32.0

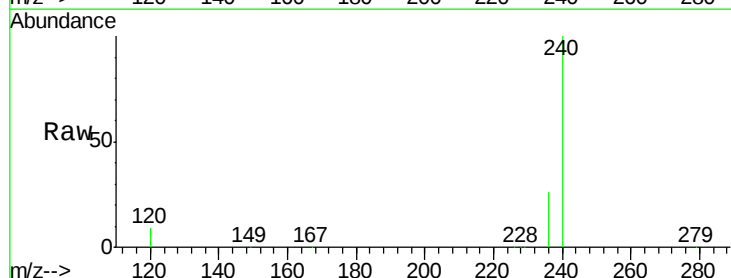


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



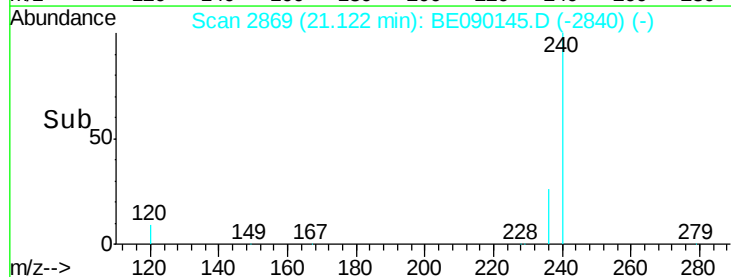
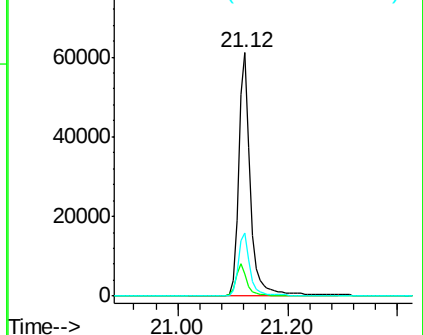


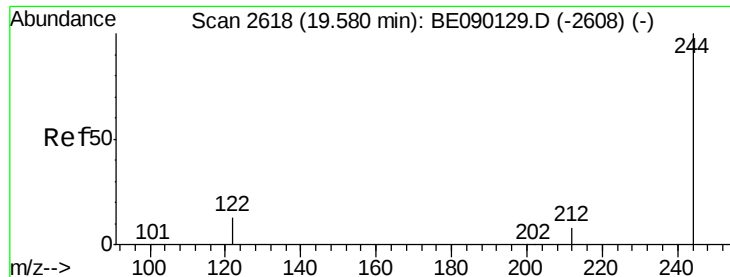

#27  
 Terphenyl-d14  
 Concen: 4.06 ng  
 RT: 19.58 min Scan# 2619  
 Delta R.T. 0.00 min  
 Lab File: BE090145.D  
 Acq: 17 Jul 2015 7:42




Instrument :  
 BNA\_E  
 ClientSampleId :  
 FB-01-071515


Tgt Ion: 244 Resp: 59427  
 Ion Ratio Lower Upper  
 244 100  
 212 7.5 6.7 10.1  
 122 10.2 10.7 16.1#

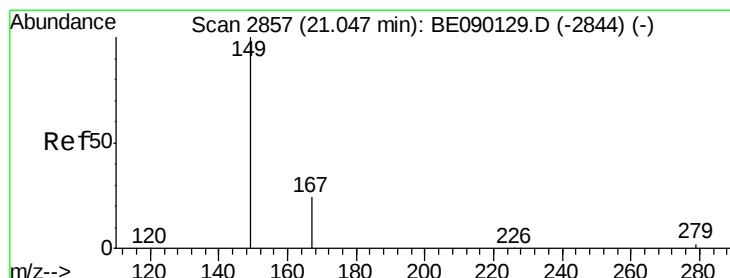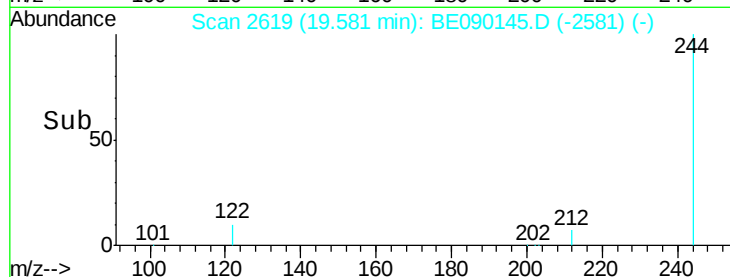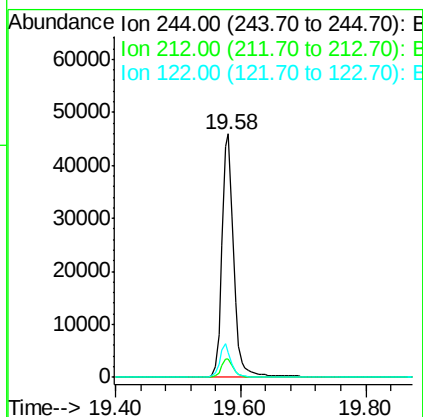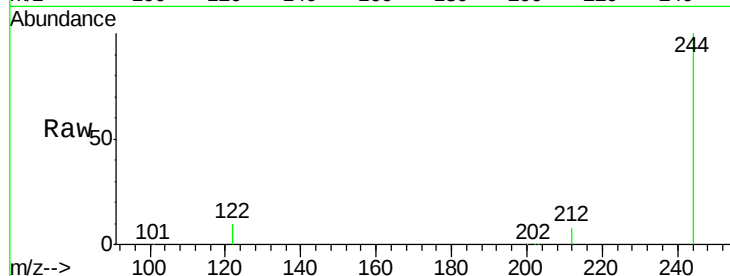

#30  
 Bis(2-ethylhexyl)phthalate  
 Concen: 0.40 ng  
 RT: 21.05 min Scan# 2858  
 Delta R.T. 0.00 min  
 Lab File: BE090145.D  
 Acq: 17 Jul 2015 7:42

Tgt Ion: 149 Resp: 1122  
 Ion Ratio Lower Upper  
 149 100  
 167 24.2 18.6 27.8  
 279 3.3 2.2 3.4

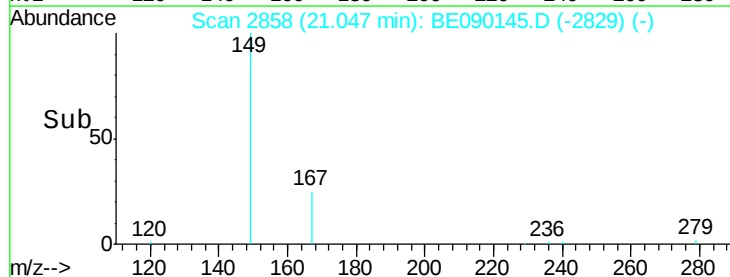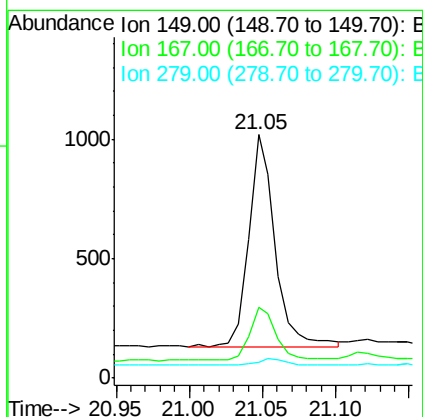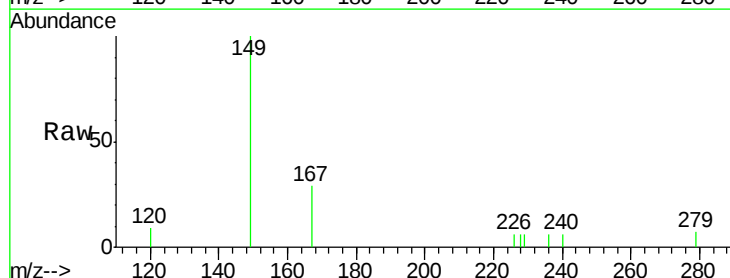

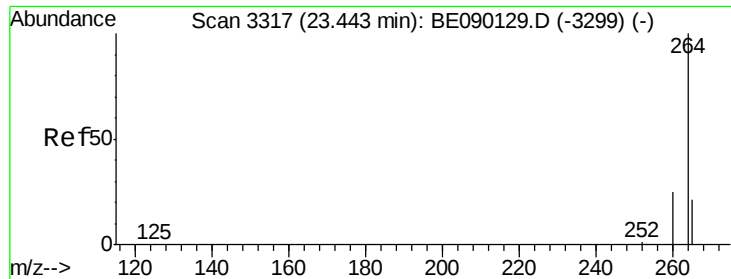

#32  
Perylene-d12  
Concen: 5.00 ng  
RT: 23.44 min Scan# 3317  
Delta R.T. -0.00 min  
Lab File: BE090145.D  
Acq: 17 Jul 2015 7:42

Instrument :  
BNA\_E  
ClientSampleId :  
FB-01-071515

Tgt Ion: 264 Resp: 78321  
Ion Ratio Lower Upper  
264 100  
260 24.7 19.9 29.9  
265 22.3 17.8 26.8

