


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE071715\
Data File : BE090150.D
Acq On : 17 Jul 2015 18:00
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE071715.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jul 18 00:40:53 2015

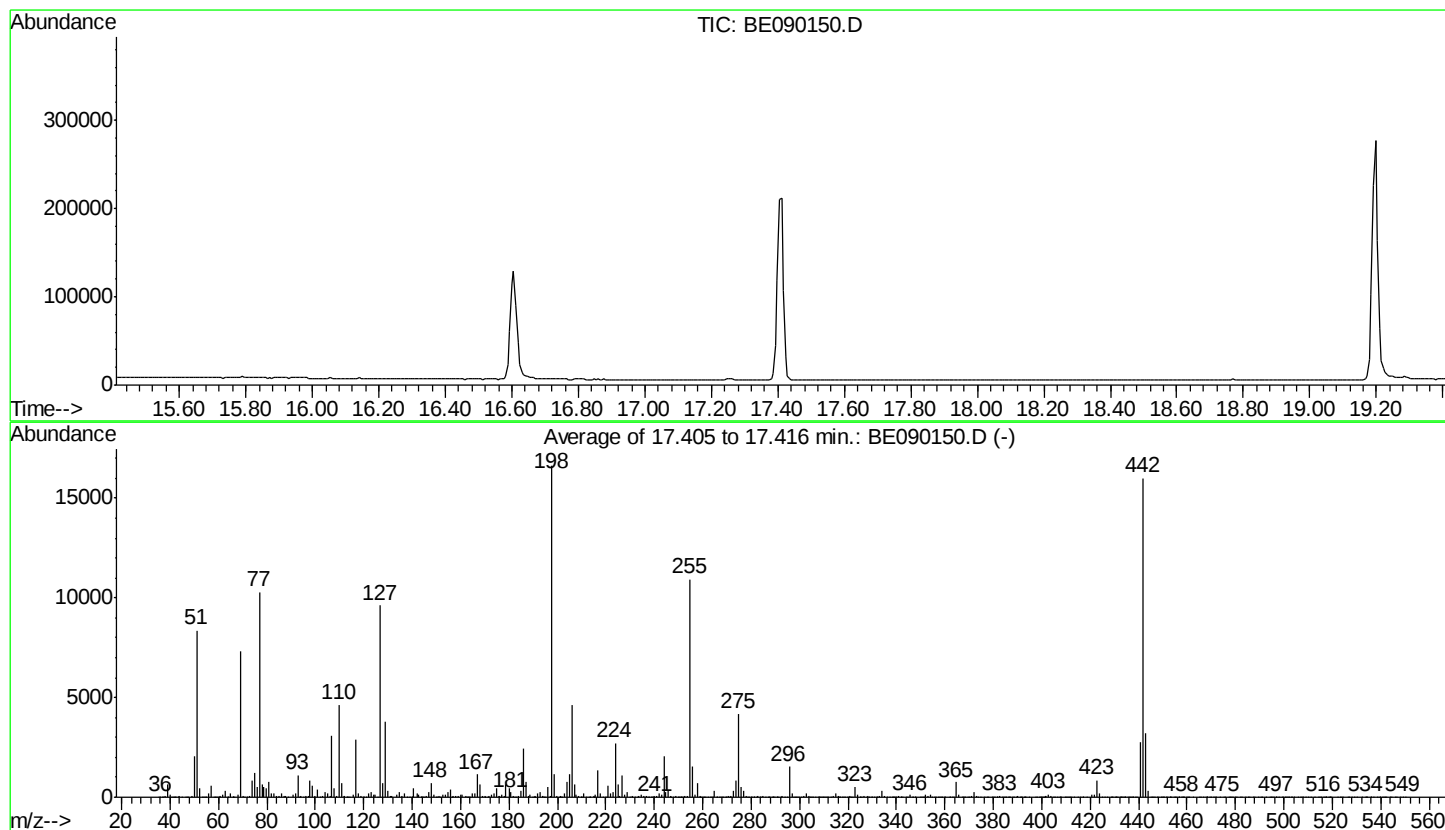

AutoFind: Scans 2522, 2523, 2524; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.3	8361	PASS
68	69	0.00	2	1.7	124	PASS
69	198	0.00	100	44.1	7338	PASS
70	69	0.00	2	0.8	59	PASS
127	198	10	80	57.8	9611	PASS
197	198	0.00	2	0.2	41	PASS
198	198	100	100	100.0	16637	PASS
199	198	5	9	7.0	1164	PASS
275	198	10	60	25.3	4205	PASS
365	198	1	100	4.5	745	PASS
441	442	0.01	24	17.1	2747	PASS
442	198	50	100	96.3	16021	PASS
443	442	15	24	19.9	3195	PASS