


Data Path : Z:\HPCHEM1\BNA_E\DATA\BE071715\
Data File : BE090166.D
Acq On : 18 Jul 2015 4:10
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE071715.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jul 18 00:40:53 2015

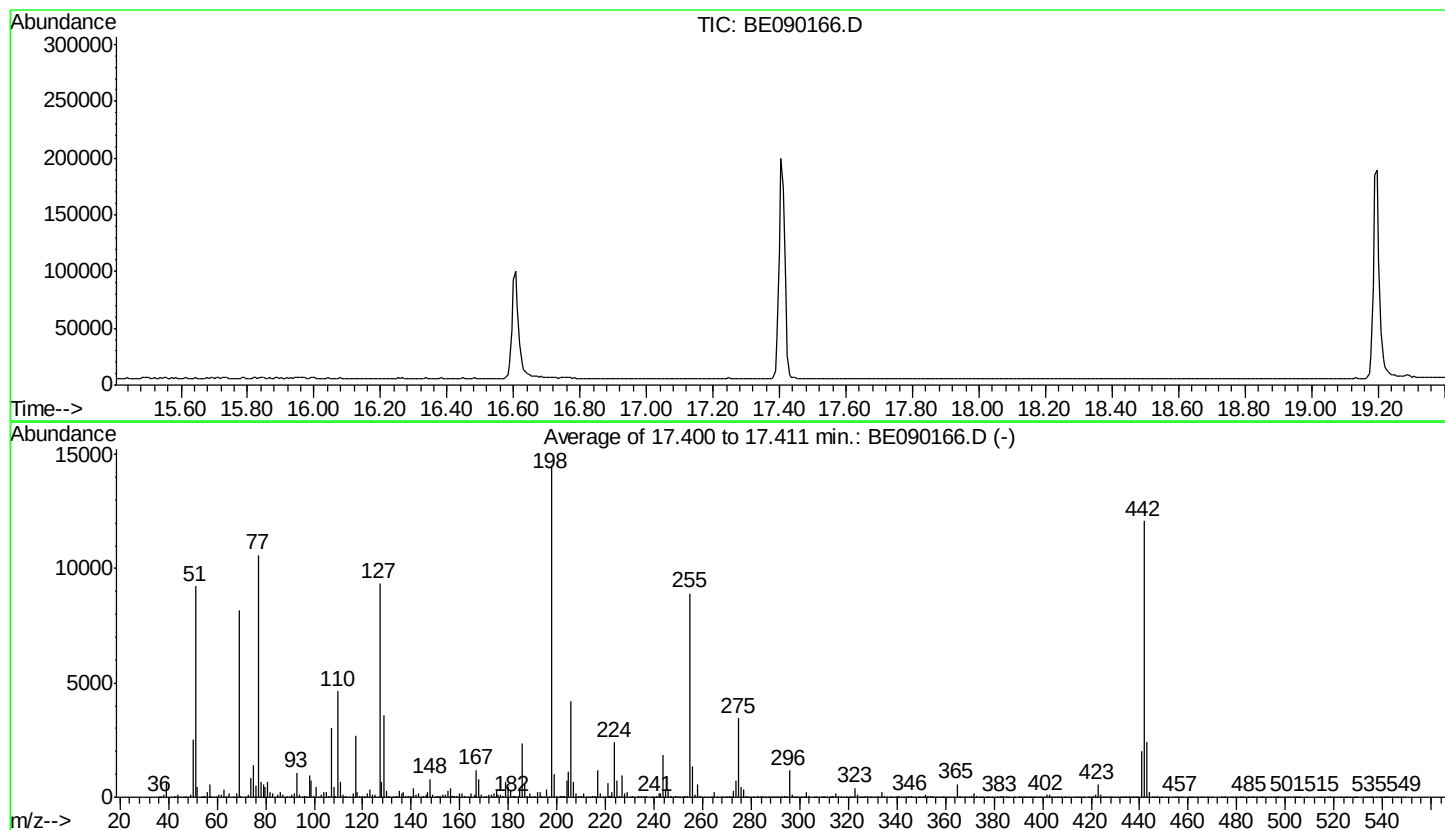

AutoFind: Scans 2521, 2522, 2523; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	63.6	9218	PASS
68	69	0.00	2	1.8	145	PASS
69	198	0.00	100	56.3	8159	PASS
70	69	0.00	2	0.5	38	PASS
127	198	10	80	64.4	9340	PASS
197	198	0.00	2	0.0	6	PASS
198	198	100	100	100.0	14501	PASS
199	198	5	9	7.0	1015	PASS
275	198	10	60	23.8	3456	PASS
365	198	1	100	4.0	586	PASS
441	442	0.01	24	16.8	2023	PASS
442	198	50	100	83.2	12070	PASS
443	442	15	24	19.9	2396	PASS