


Data Path : Z:\HPCHEM1\BNA E\Data\BE071917\
 Data File : BE093476.D
 Acq On : 19 Jul 2017 8:58
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE070217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 03 06:40:23 2017

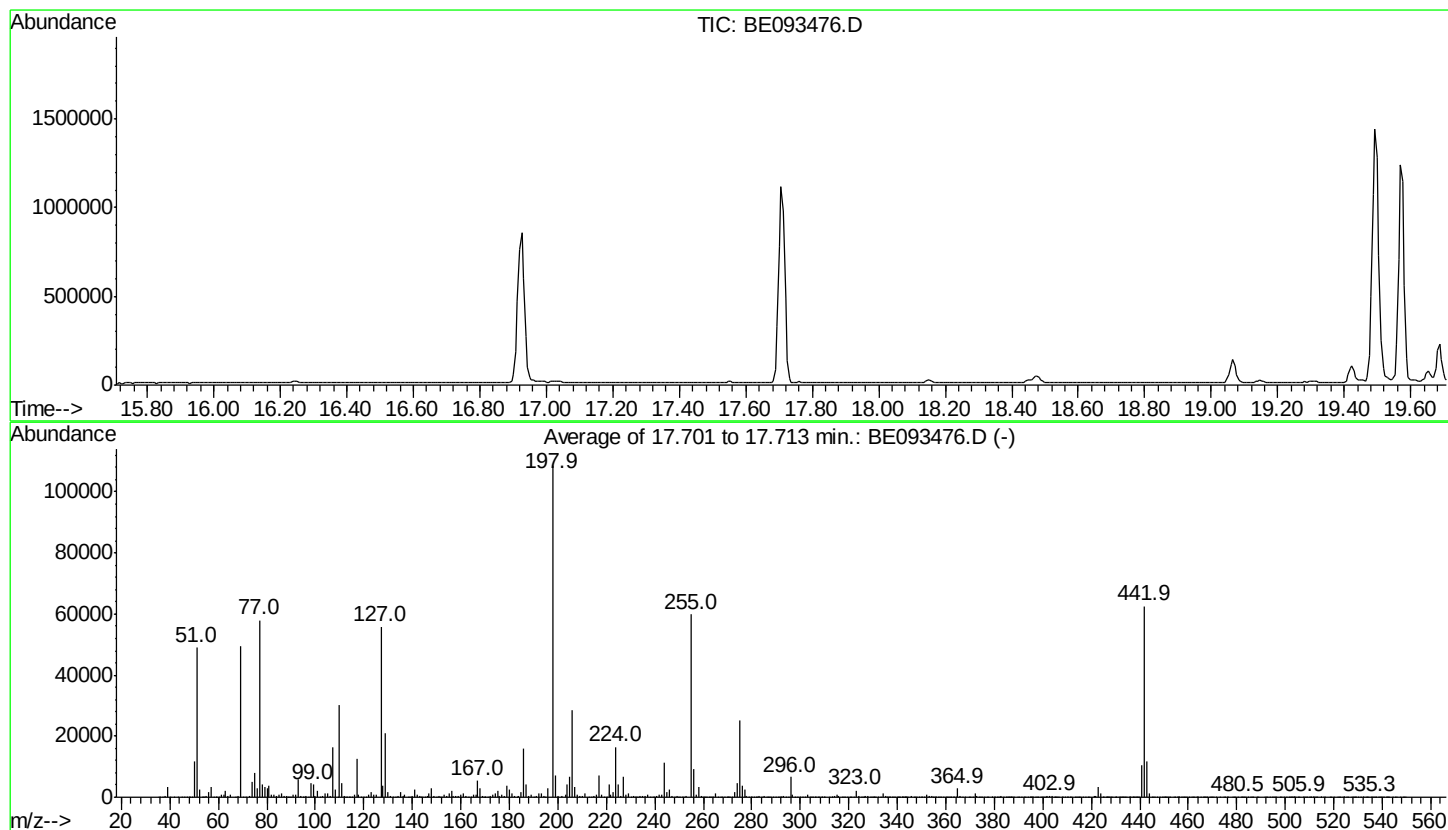

AutoFind: Scans 2572, 2573, 2574; Background Corrected with Scan 2562

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	48955	PASS
68	69	0.00	2	0.5	252	PASS
69	198	0.00	100	45.4	49324	PASS
70	69	0.00	2	0.4	191	PASS
127	198	10	80	51.5	55885	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	108586	PASS
199	198	5	9	6.7	7269	PASS
275	198	10	60	23.3	25282	PASS
365	198	1	100	2.6	2813	PASS
441	442	0.01	24	16.6	10367	PASS
442	198	50	100	57.5	62461	PASS
443	442	15	24	19.1	11913	PASS