


Data Path : S:\HPCHEM1\BNA_E\Data\BE072015\
 Data File : BE090174.D
 Acq On : 20 Jul 2015 13:13
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : S:\HPCHEM1\BNA_E\METHODS\8270-SIM-BE071715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Jul 18 00:40:53 2015

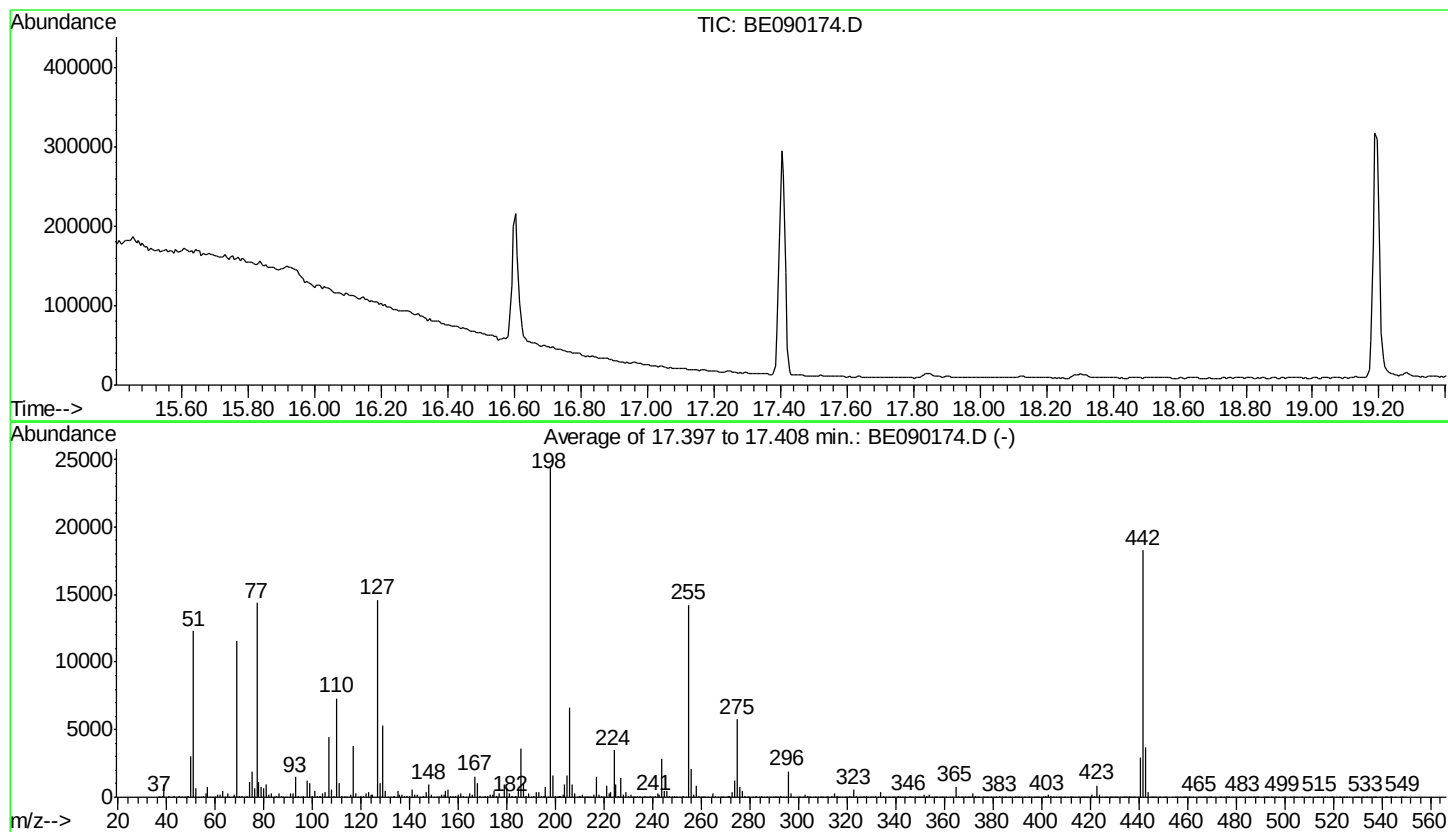

AutoFind: Scans 2520, 2521, 2522; Background Corrected with Scan 2514

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.1	12285	PASS
68	69	0.00	2	1.9	216	PASS
69	198	0.00	100	47.1	11542	PASS
70	69	0.00	2	0.5	59	PASS
127	198	10	80	59.5	14603	PASS
197	198	0.00	2	0.2	45	PASS
198	198	100	100	100.0	24528	PASS
199	198	5	9	6.5	1590	PASS
275	198	10	60	23.4	5740	PASS
365	198	1	100	3.2	784	PASS
441	442	0.01	24	16.1	2940	PASS
442	198	50	100	74.3	18235	PASS
443	442	15	24	20.5	3734	PASS