

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072115\
 Data File : BE090190.D
 Acq On : 21 Jul 2015 00:22
 Operator : TP/IZ
 Sample : MDL-05-W
 Misc : MDL-WATER-SIM2.2-0.07PPM
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: Jul 21 05:23:12 2015

Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE072115.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Jul 21 05:15:45 2015

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	943	0.40	ng/ul	0.00
2) Naphthalene-d8	10.37	136	4531	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.22	164	2610	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.95	188	7031	0.40	ng/ul	0.01
16) Chrysene-d12	21.12	240	6486	0.40	ng/ul	0.00
20) Perylene-d12	23.43	264	4971	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.96	152	2742	0.38	ng/ul	0.00
14) Fluoranthene-d10	18.98	212	8233	0.39	ng/ul	0.00


Target Compounds


						Qvalue
3) Naphthalene	10.42	128	641	0.05	ng/ul#	78
5) 2-Methylnaphthalene	12.03	142	414	0.05	ng/ul	94
7) Acenaphthylene	13.93	152	3025	0.06	ng/ul#	86
8) Acenaphthene	14.27	153	2147	0.05	ng/ul	93
9) Fluorene	15.27	166	658	0.06	ng/ul#	94
11) Pentachlorophenol	16.62	266	1	0.00	ng/ul#	21
12) Phenanthrene	16.99	178	4411	0.05	ng/ul#	88
13) Anthracene	17.07	178	4259	0.05	ng/ul#	84
15) Fluoranthene	19.00	202	5275	0.05	ng/ul	88
17) Pyrene	19.36	202	5384	0.07	ng/ul#	93
18) Benzo(a)anthracene	21.10	228	632	0.04	ng/ul#	83
19) Chrysene	21.15	228	1234	0.06	ng/ul#	88
21) Benzo(b)fluoranthene	22.73	252	392	0.03	ng/ul#	51
22) Benzo(k)fluoranthene	22.77	252	654	0.04	ng/ul#	58
23) Benzo(a)pyrene	23.33	252	461	0.03	ng/ul#	42
24) Indeno(1,2,3-cd)pyrene	25.83	276	1407	0.02	ng/ul	97
25) Dibenzo(a,h)anthracene	25.85	278	232	0.02	ng/ul#	27
26) Benzo(g,h,i)perylene	26.56	276	1860	0.03	ng/ul#	54

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_E\DATA\BE072115\
Data File : BE090190.D
Acq On : 21 Jul 2015 00:22
Operator : TP/IZ
Sample : MDL-05-W
Misc : MDL-WATER-SIM2.2-0.07PPM
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Jul 21 05:23:12 2015
Quant Method : Z:\HPCHEM1\BNA_E\METHODS\SOM02.2-EPA-SIM-BE072115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 21 05:15:45 2015
Response via : Initial Calibration

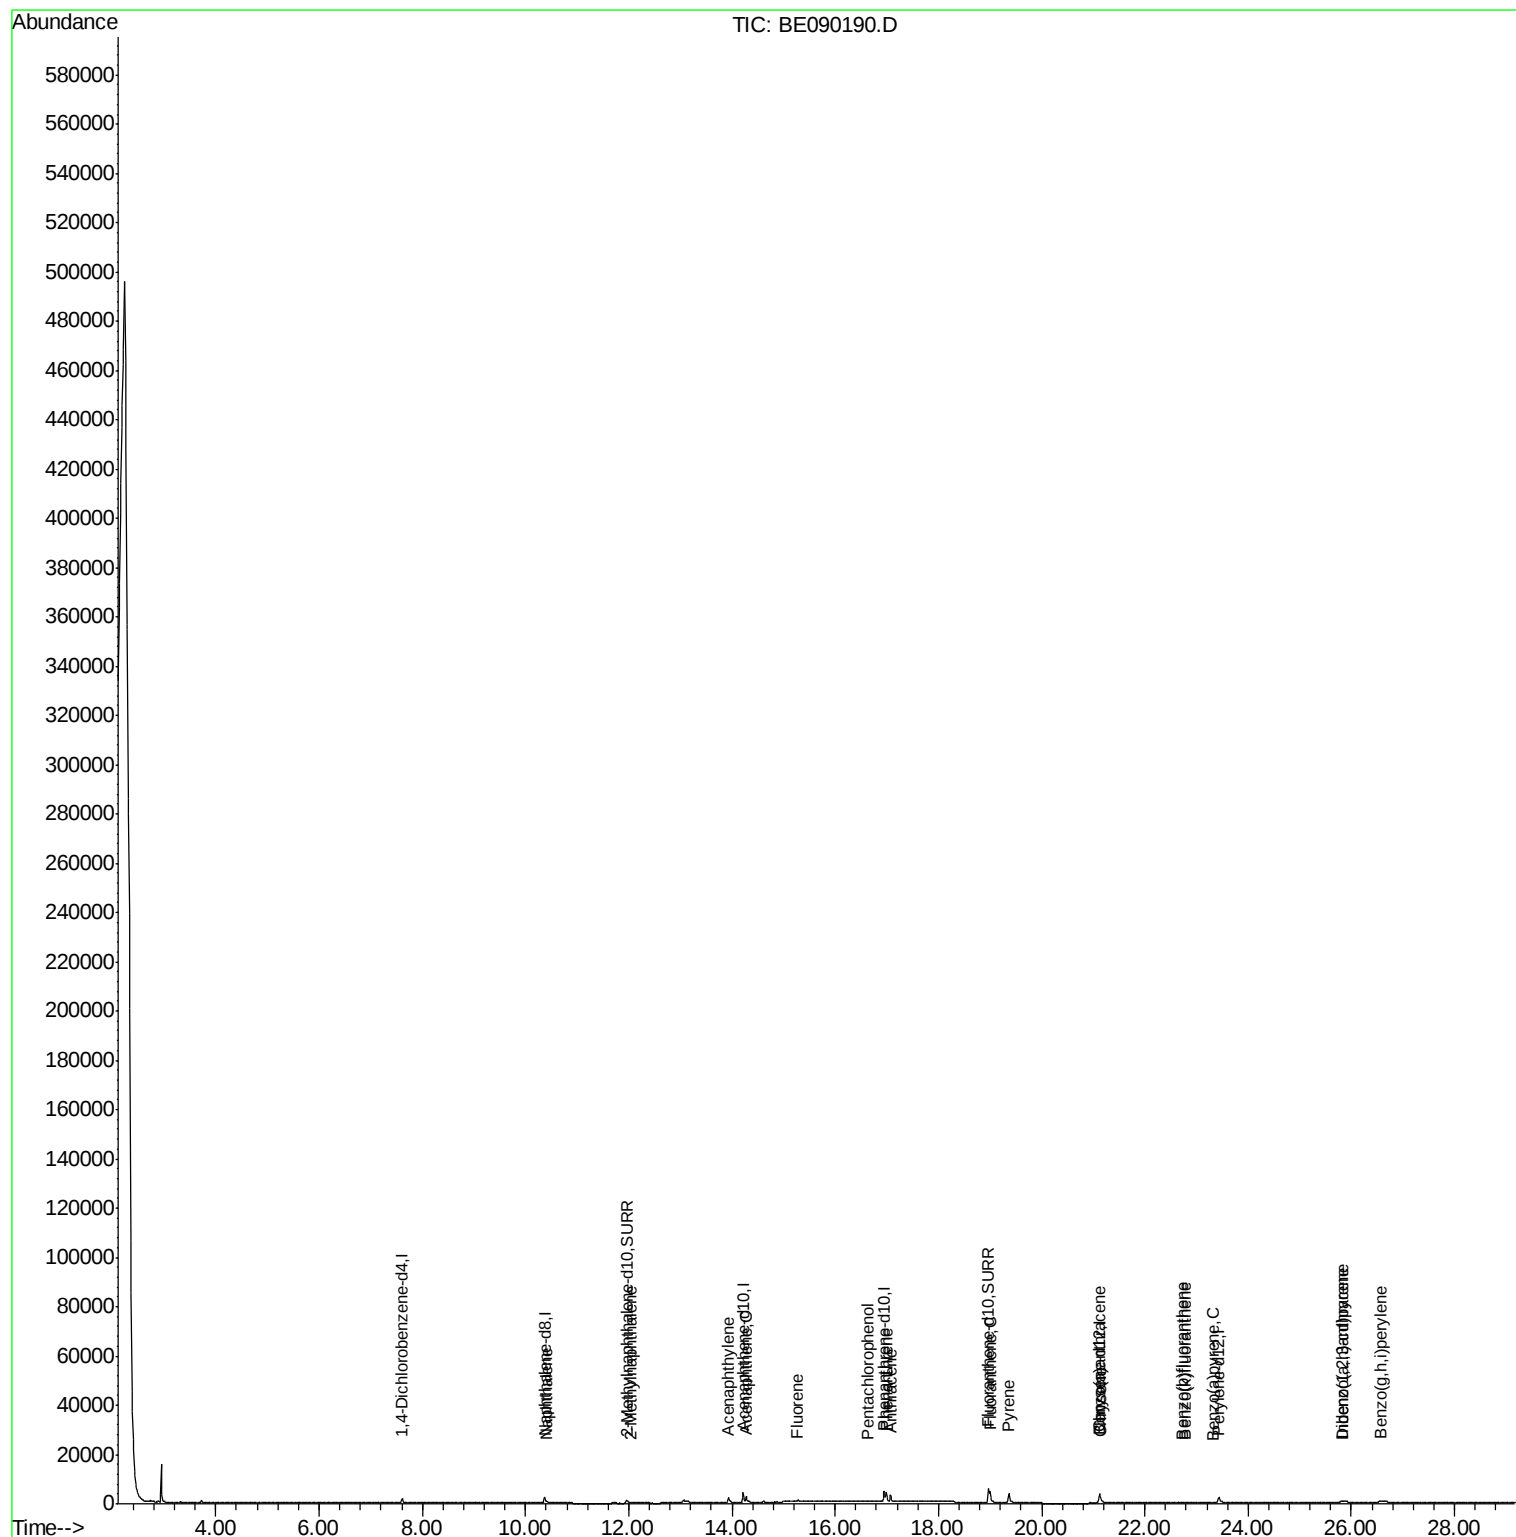



#3

Naphthalene

Concen: 0.05 ng/ul

RT: 10.42 min Scan# 1294

Delta R.T. 0.00 min

Lab File: BE090190.D

Acq: 21 Jul 2015 00:22


Tgt Ion:128 Resp: 641

Ion Ratio Lower Upper

128 100

129 22.1 10.2 15.4#

127 23.2 11.9 17.9#



Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

10.42

400



300

200

100

0

Time-->

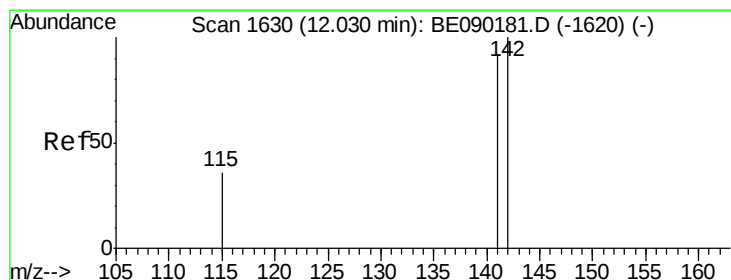

#5

2-Methylnaphthalene

Concen: 0.05 ng/ul

RT: 12.03 min Scan# 1630

Delta R.T. -0.00 min

Lab File: BE090190.D


Acq: 21 Jul 2015 00:22

Tgt Ion:142 Resp: 414

Ion Ratio Lower Upper

142 100

141 97.8 73.4 110.2

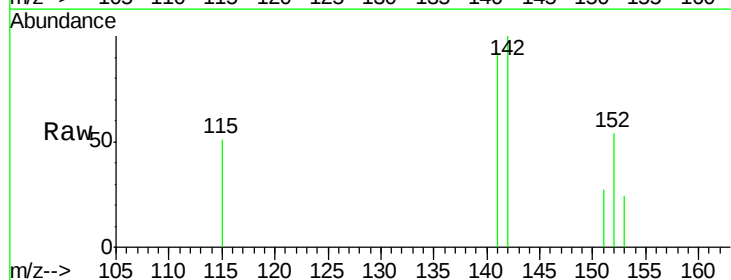

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

12.03

250

200


150


100

50

0

Time-->





#7

Acenaphthylene

Concen: 0.06 ng/ul

RT: 13.93 min Scan# 1905

Delta R.T. -0.00 min

Lab File: BE090190.D

Acq: 21 Jul 2015 00:22


Tgt Ion:152 Resp: 3025

Ion Ratio Lower Upper




152 100

151 7.4 4.2 6.4#

153 22.1 11.9 17.9#



Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E
Ion 153.00 (152.70 to 153.70): E

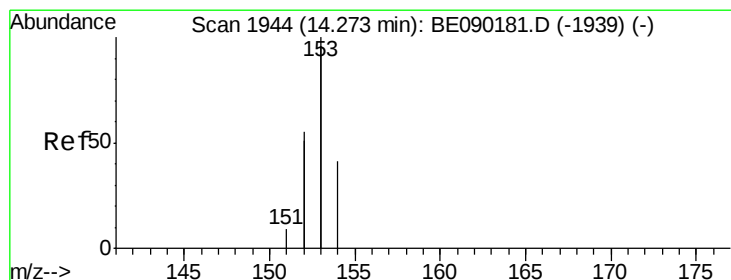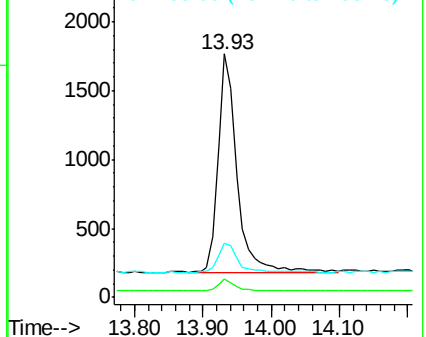

#8

Acenaphthene

Concen: 0.05 ng/ul

RT: 14.27 min Scan# 1944

Delta R.T. -0.00 min

Lab File: BE090190.D

Acq: 21 Jul 2015 00:22


Tgt Ion:153 Resp: 2147

Ion Ratio Lower Upper



153 100


152 61.8 43.8 65.8

154 21.5 16.8 25.2







Abundance Ion 153.00 (152.70 to 153.70): E
Ion 152.00 (151.70 to 152.70): E
Ion 154.00 (153.70 to 154.70): E

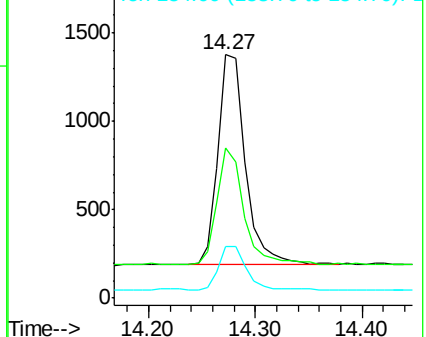






#9
Fluorene
 Concen: 0.06 ng/ul
 RT: 15.27 min Scan# 2058
 Delta R.T. 0.01 min
 Lab File: BE090190.D
 Acq: 21 Jul 2015 00:22


Tgt Ion:166 Resp: 658
 Ion Ratio Lower Upper
 166 100
 165 99.2 81.2 121.8
 167 27.1 12.6 19.0#

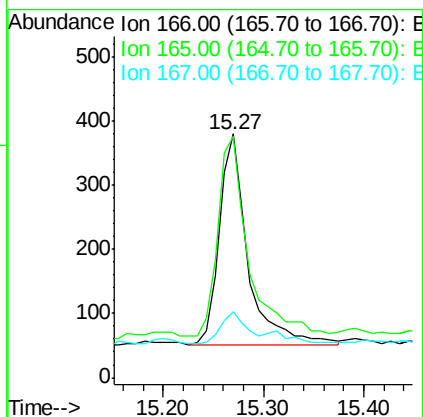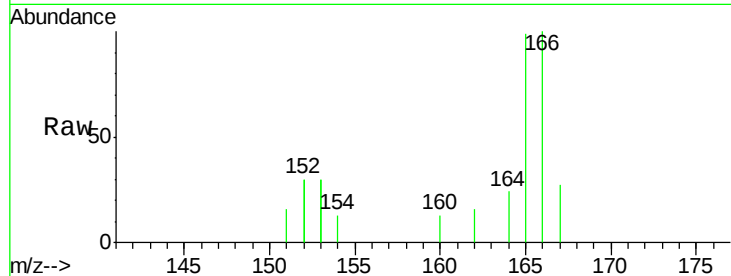

#11
Pentachlorophenol
 Concen: 0.00 ng/ul
 RT: 16.62 min Scan# 2188
 Delta R.T. 0.01 min
 Lab File: BE090190.D
 Acq: 21 Jul 2015 00:22


Tgt Ion:266 Resp: 1
 Ion Ratio Lower Upper
 266 100
 264 0.0 47.7 71.5#
 268 0.0 47.0 70.6#

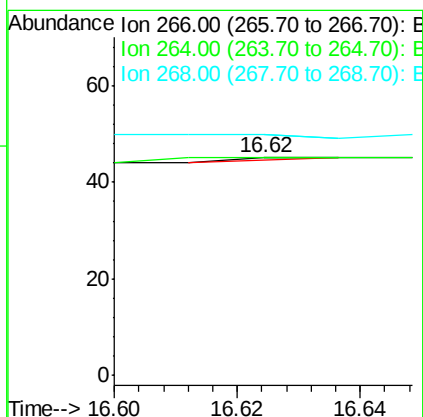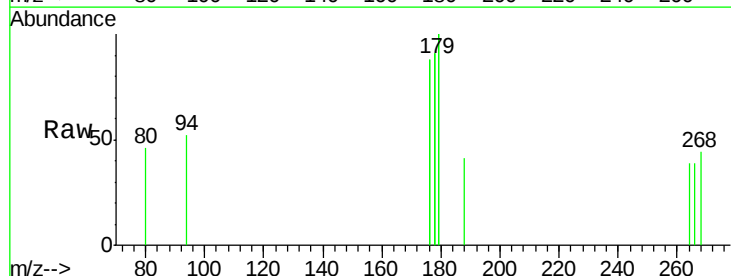



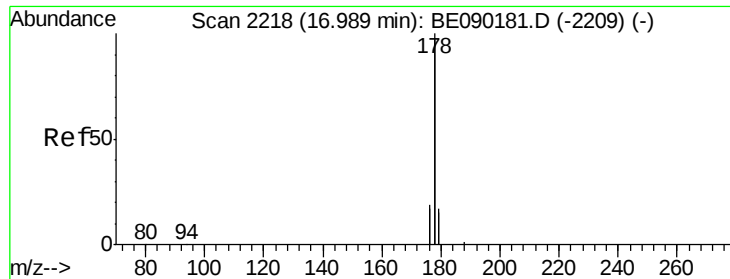


#12
Phenanthrene
Concen: 0.05 ng/ul
RT: 16.99 min Scan# 2218
Delta R.T. -0.00 min
Lab File: BE090190.D
Acq: 21 Jul 2015 00:22

Tgt Ion:178 Resp: 4411
Ion Ratio Lower Upper
178 100
176 24.3 15.3 22.9#
179 22.9 14.0 21.0#

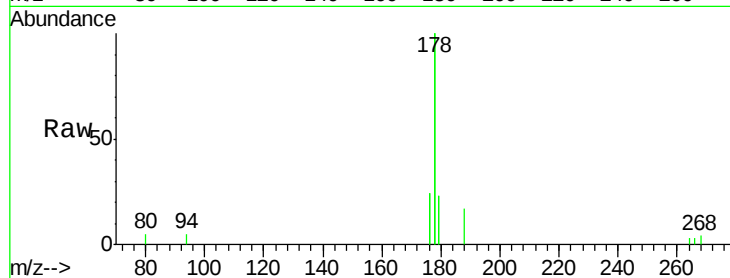


Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

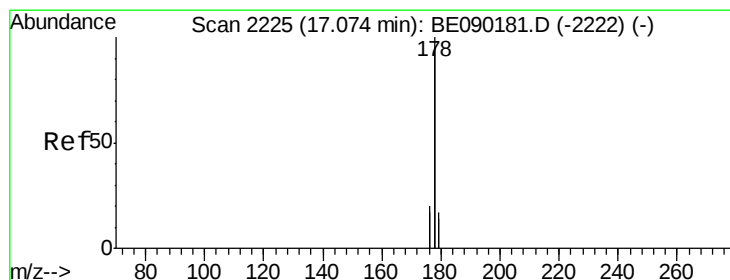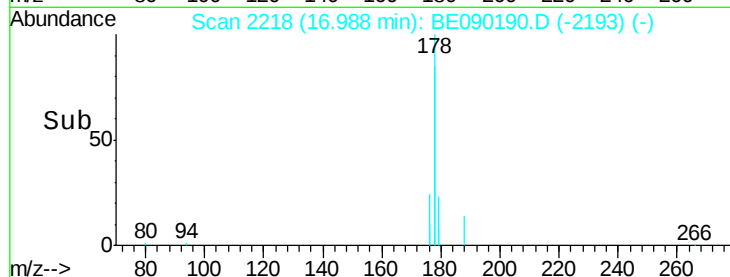
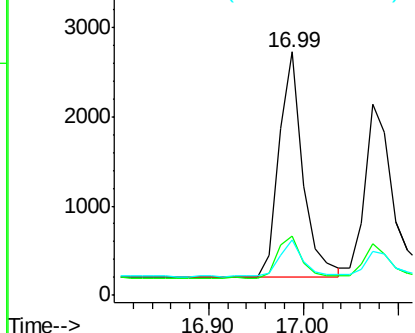



#13
Anthracene
Concen: 0.05 ng/ul
RT: 17.07 min Scan# 2225
Delta R.T. -0.00 min
Lab File: BE090190.D
Acq: 21 Jul 2015 00:22

Tgt Ion:178 Resp: 4259
Ion Ratio Lower Upper
178 100
176 27.3 16.0 24.0#
179 23.2 13.4 20.0#

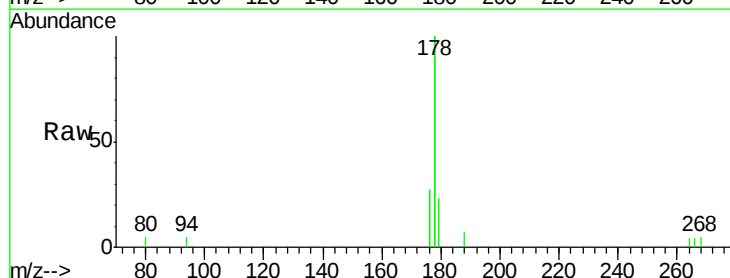





Abundance Ion 178.00 (177.70 to 178.70): E
Ion 176.00 (175.70 to 176.70): E
Ion 179.00 (178.70 to 179.70): E

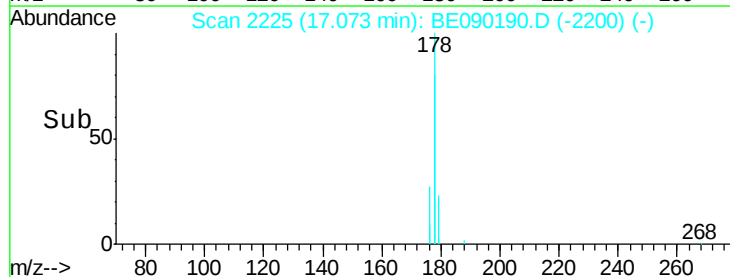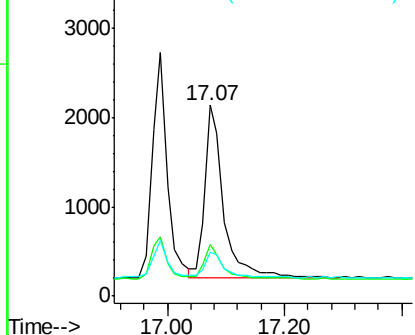






#15
Fluoranthene
 Concen: 0.05 ng/ul
 RT: 19.00 min Scan# 2430
 Delta R.T. 0.01 min
 Lab File: BE090190.D
 Acq: 21 Jul 2015 00:22


Tgt Ion: 202 Resp: 5275
 Ion Ratio Lower Upper
 202 100
 101 4.0 0.0 23.0
 203 23.0 0.0 37.0

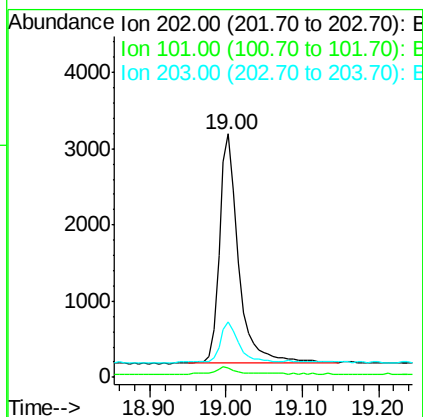

#17
Pyrene
 Concen: 0.07 ng/ul
 RT: 19.36 min Scan# 2485
 Delta R.T. -0.00 min
 Lab File: BE090190.D
 Acq: 21 Jul 2015 00:22





Tgt Ion: 202 Resp: 5384
 Ion Ratio Lower Upper
 202 100
 200 6.6 4.3 6.5#
 203 21.9 14.6 21.8#

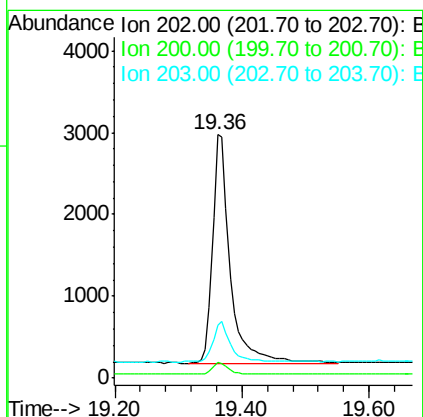

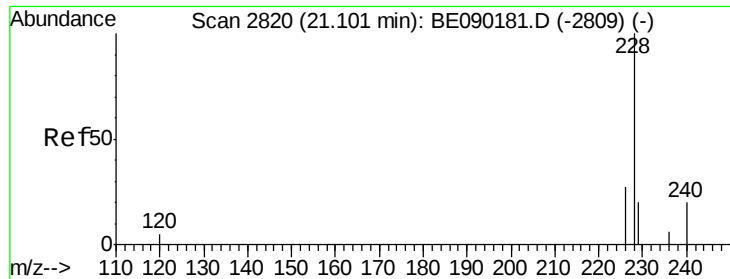




#18
Benzo(a)anthracene
Concen: 0.04 ng/ul
RT: 21.10 min Scan# 2821
Delta R.T. 0.00 min
Lab File: BE090190.D
Acq: 21 Jul 2015 00:22


Tgt Ion:228 Resp: 632
Ion Ratio Lower Upper
228 100
226 36.3 22.2 33.4#
229 29.9 16.9 25.3#

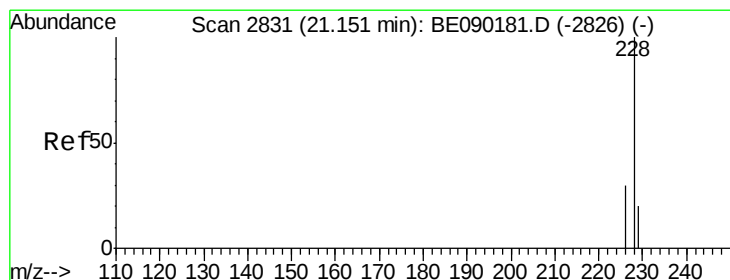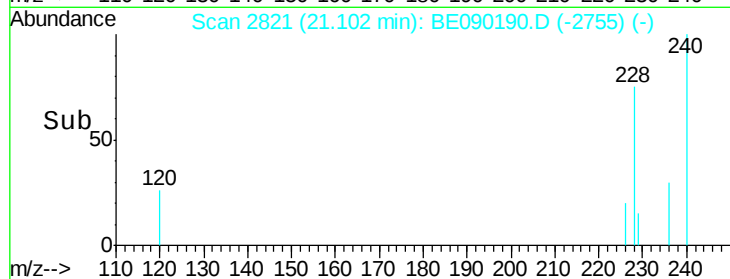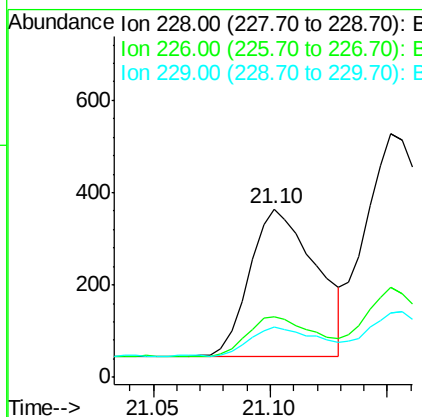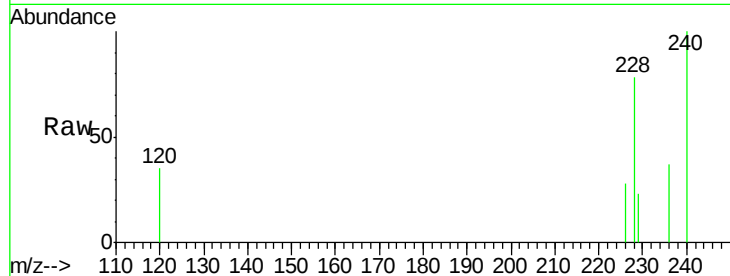

#19
Chrysene
Concen: 0.06 ng/ul
RT: 21.15 min Scan# 2832
Delta R.T. 0.00 min
Lab File: BE090190.D
Acq: 21 Jul 2015 00:22

Tgt Ion:228 Resp: 1234
Ion Ratio Lower Upper
228 100
226 37.2 24.3 36.5#
229 26.2 16.6 24.8#

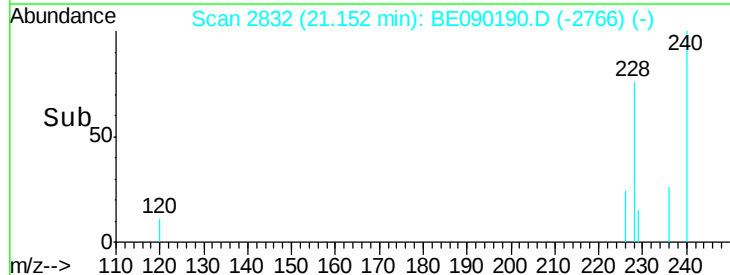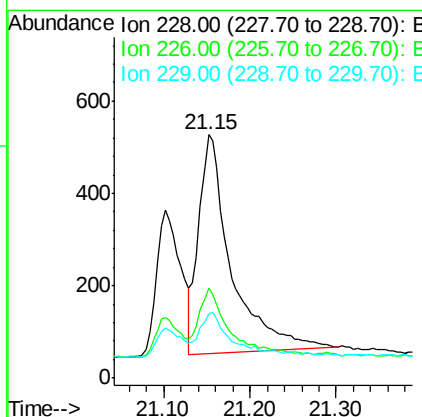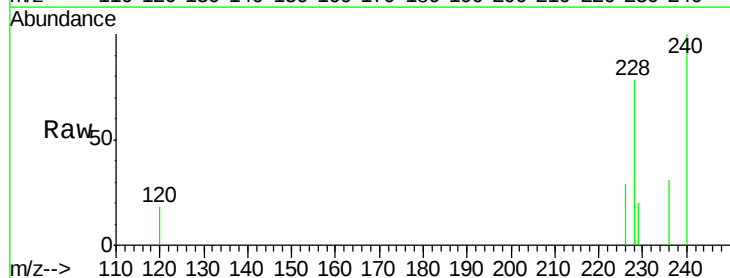



#21

Benzo(b)fluoranthene

Concen: 0.03 ng/ul





RT: 22.73 min Scan# 3174

Delta R.T. 0.00 min

Lab File: BE090190.D

Acq: 21 Jul 2015 00:22

Tgt Ion:	252	Resp:	392
Ion	Ratio	Lower	Upper
252	100		
253	42.3	0.0	46.8
125	39.8	0.0	25.4#

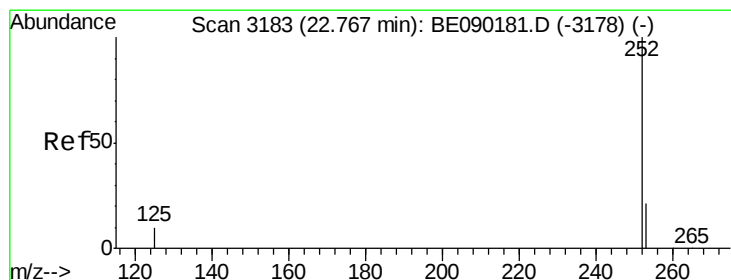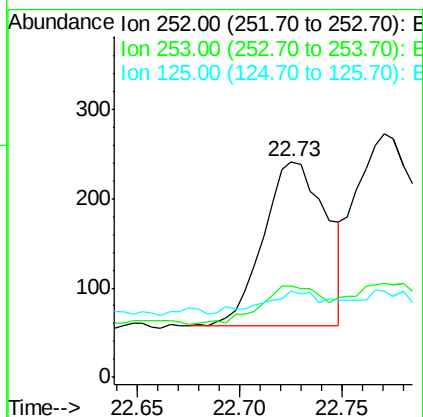

#22

Benzo(k)fluoranthene

Concen: 0.04 ng/ul




RT: 22.77 min Scan# 3184


Delta R.T. 0.00 min

Lab File: BE090190.D

Acq: 21 Jul 2015 00:22

Tgt Ion:	252	Resp:	654
Ion	Ratio	Lower	Upper
252	100		
253	38.6	18.3	27.5#
125	35.3	9.8	14.8#

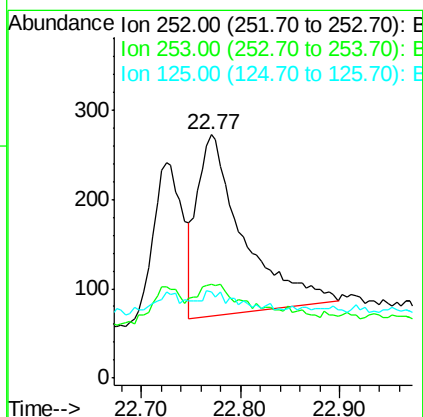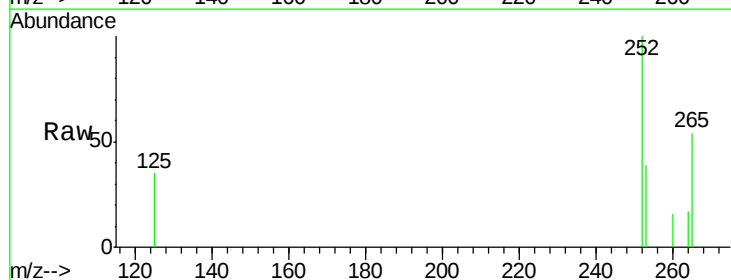



#23

Benzo(a)pyrene

Concen: 0.03 ng/ul

RT: 23.33 min Scan# 3306

Delta R.T. 0.00 min

Lab File: BE090190.D

Acq: 21 Jul 2015 00:22


Tgt Ion: 252 Resp: 461

Ion Ratio Lower Upper




252 100

253 46.4 18.4 27.6#

125 44.4 11.5 17.3#



Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

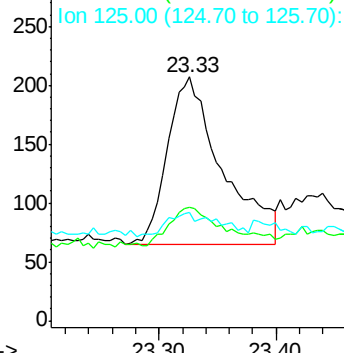

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.02 ng/ul

RT: 25.83 min Scan# 3797

Delta R.T. 0.00 min

Lab File: BE090190.D

Acq: 21 Jul 2015 00:22


Tgt Ion: 276 Resp: 1407

Ion Ratio Lower Upper



276 100


138 23.8 19.8 29.8

277 22.9 19.8 29.6



Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E




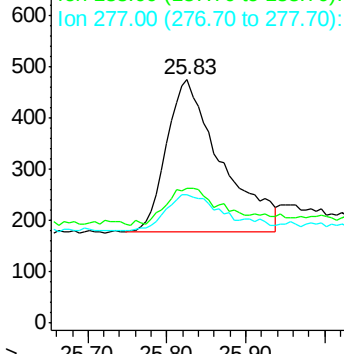




#25
Dibenzo(a,h)anthracene
Concen: 0.02 ng/ul
RT: 25.85 min Scan# 3800
Delta R.T. 0.00 min
Lab File: BE090190.D
Acq: 21 Jul 2015 00:22

Tgt Ion: 278 Resp: 232

Ion	Ratio	Lower	Upper
278	100		
139	0.0	0.0	0.0
279	61.6	20.0	30.0#

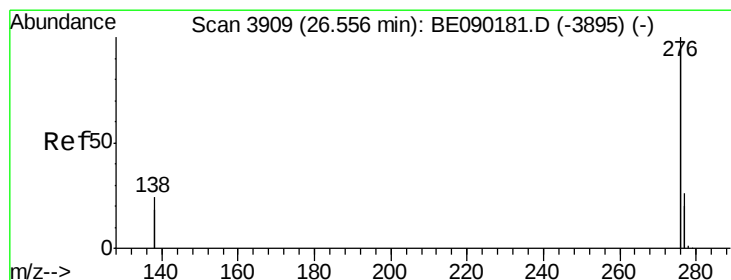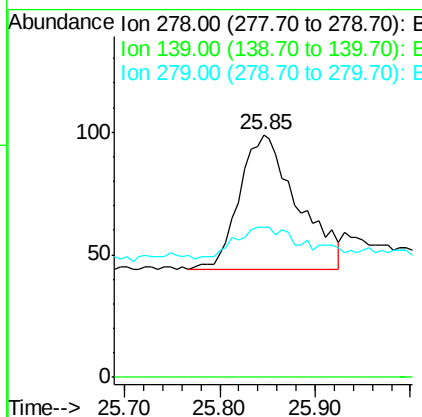

#26
Benzo(g,h,i)perylene
Concen: 0.03 ng/ul
RT: 26.56 min Scan# 3910
Delta R.T. 0.01 min
Lab File: BE090190.D
Acq: 21 Jul 2015 00:22

Tgt Ion: 276 Resp: 1860

Ion	Ratio	Lower	Upper
276	100		
277	47.2	20.6	31.0#
138	48.6	19.3	28.9#

